

Water, Food & Environmental Analytics

Test Kits, Instruments and Accessories



The life science business of Merck operates as MilliporeSigma in the U.S. and Canada.

MERCK

Merck Millipore + Sigma Aldrich = The Life Science business of Merck

The life science business of Merck KGaA, Darmstadt, Germany brings together the world-class products and services, innovative capabilities and exceptional talent of Merck Millipore and Sigma-Aldrich to create a global leader in the life science industry. Our exciting transformation is reflected in our striking new design. Bold and distinctive, intriguing and imaginative, warm and confident. **It shows you exactly what you can expect from Merck: a bright future.**


WE ARE A LEADER IN LIFE SCIENCE

We aim to solve the toughest problems in the industry and environments by collaborating with the global scientific community. **We provide** scientists and environmental experts with best-in-class lab materials, technologies and services. **We are dedicated** to making water, food and environmental analysis simpler, faster and more successful.



Our lively logo

We only have one Merck logo. But it can have 8 different, brilliant colors.

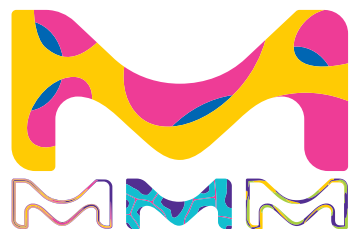

Our vibrant M

Our vibrant M is not a logo. It's a symbol that unites all our businesses, including those in the USA and Canada. So you'll always know that you're experiencing Merck's vibrant science and technology.

THIRSTY FOR CLEAN WATER

We have been leading fast, precise water analysis for more than 100 years. From A for arsenic to Z for zinc, our devices and test kits allow you to analyze virtually any substance. Whether in pipes, bottles or lakes, we help you test water with the utmost precision to make sure it's safe to sip, slurp or splash in.

HUNGRY FOR FOOD SAFETY

Our instruments, reagents and certified reference standards help you accurately monitor food quality in compliance with international regulations. So wherever, whenever someone bites into your product, they experience nothing but joy.

Life Science Facts & Figures



Our core strengths:



Comprehensive portfolio and customer-focused innovation



Balanced geographic reach



Well-differentiated, industry-leading capabilities

contents

Application Workflows



Cooling & boiler water workflow
> Page 20



Wastewater workflow
> Page 22



Drinking water workflow
> Page 24



Bottled water workflow
> Page 26



Brewery workflow
> Page 28




Food & beverage workflow
> Page 30

Parameters from A-Z	Visual and instrumental test kits at a glance		6
Photometry	Safety in water analysis Spectroquant®		32
Turbidity measurements	Get clarity in any water Turbiquant®		108
Reflectometry	Easy in-process monitoring Reflectoquant®		114
Colorimetric and titrimetric test kits	Variety and ease of use MColortest™		122
Test strips	Universal, fast and simple MQuant™		138
pH test strips and papers	pH determination made easy MColorpHast™		148
Complementary products	Be ready for anything Analysis and monitoring		154
Service	Ask for more Useful information from A-Z Product number index		164

Measuring ranges at a glance

Water and food analytics product portfolio

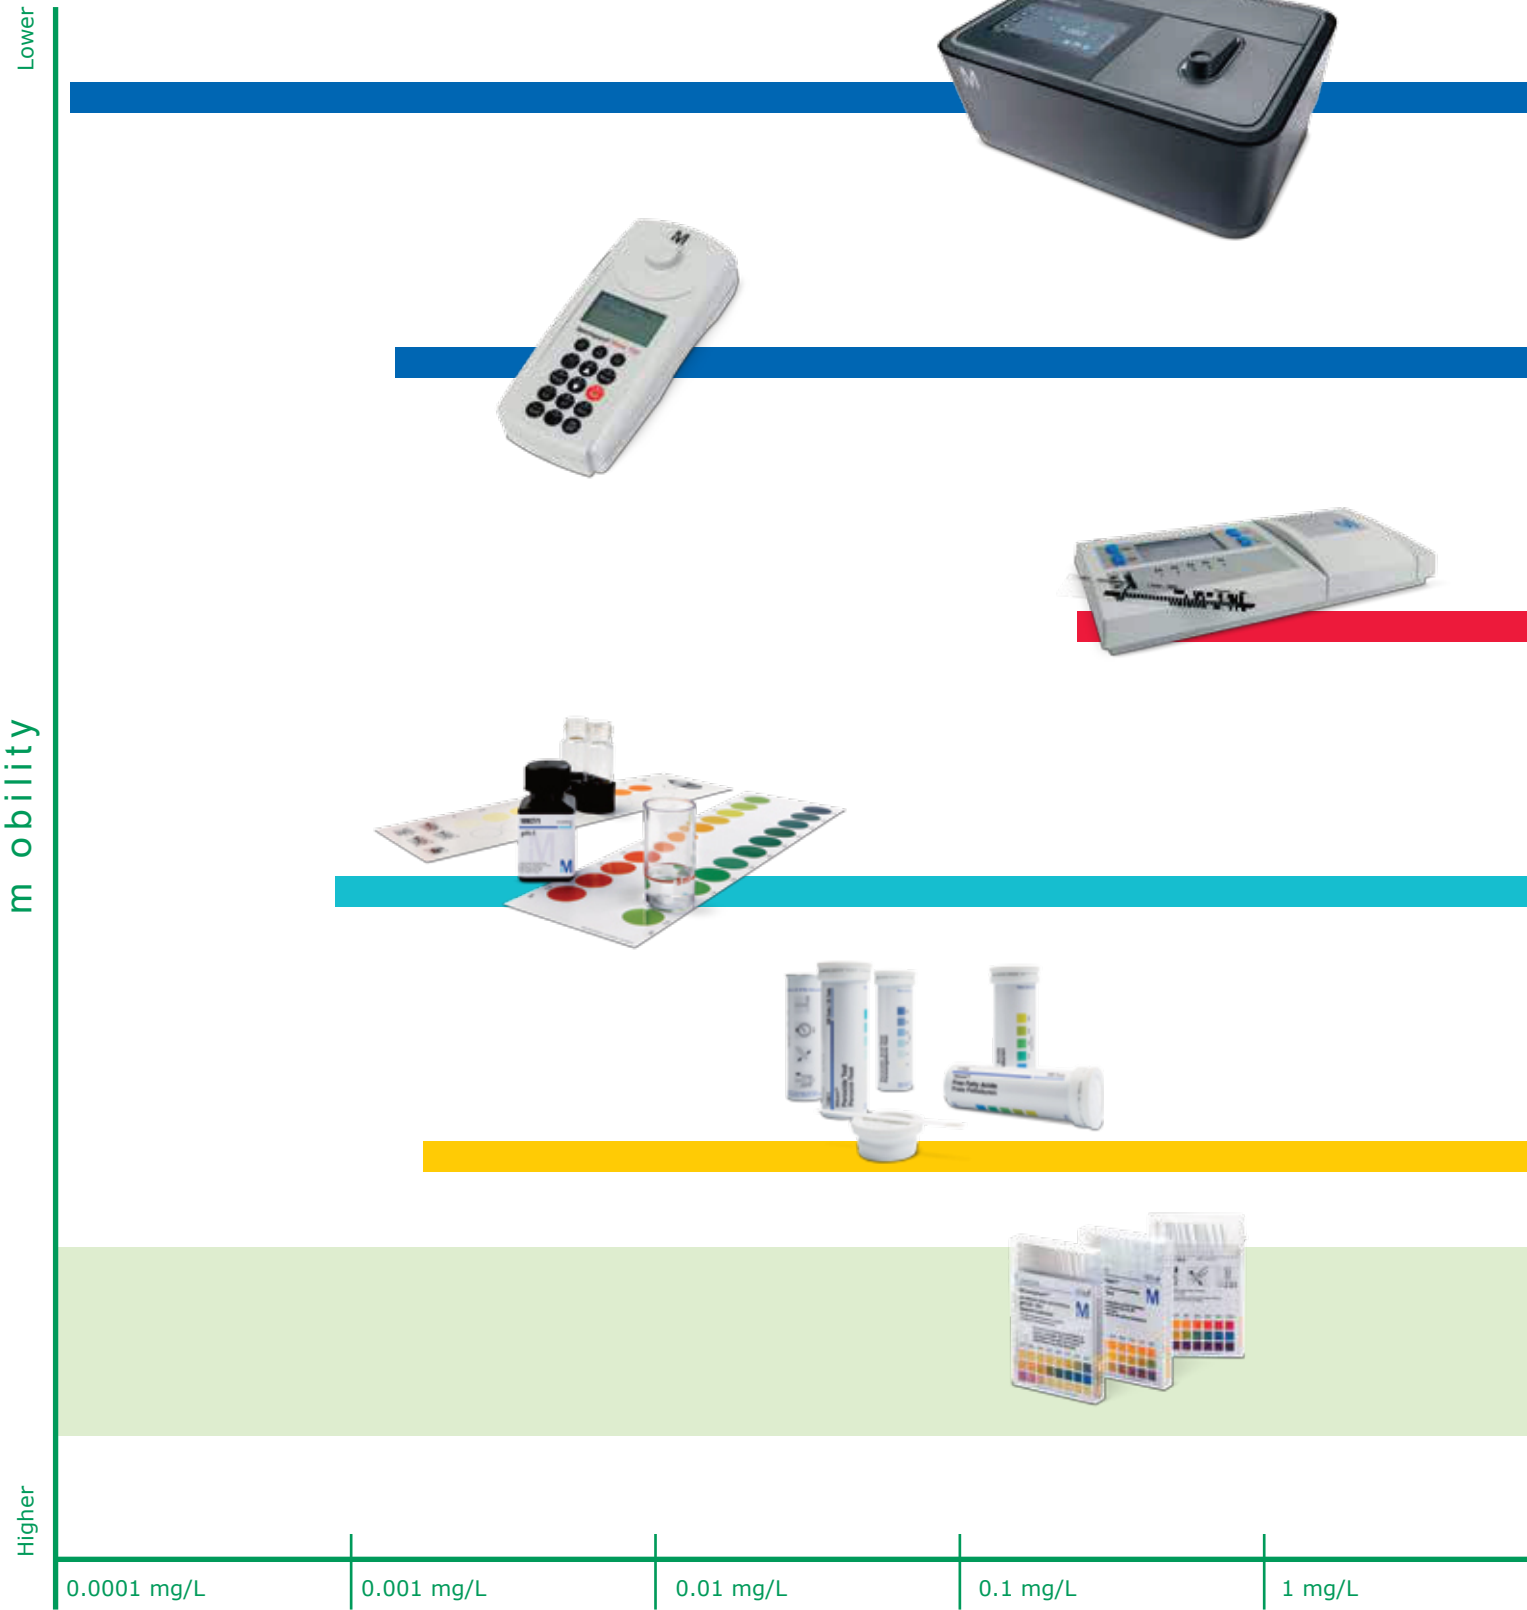



Spectroquant® Prove

www.merckmillipore.com/photometry

Secure and durable spectrophotometers with over 200 test kits for easy analysis of wastewater, drinking water or process water

> **Page 36**

0.00025 mg/L – 90,000 mg/L



Spectroquant® Move 100

www.merckmillipore.com/photometry

Small, portable colorimeter for fast, reliable on-site analysis of every important parameter for drinking and wastewater

> **Page 40**

0.004 mg/L – 90,000 mg/L



RQflex® reflectometers

www.merckmillipore.com/reflectometry

Complete system with reflectometer, test kits and strips for precise on-site quantitative analysis of critical parameters

> **Page 114**

0.2 mg/L – 2,500 mg/L



MColortest™ colorimetric test kits

www.merckmillipore.com/colorimetric-test-kits

User-friendly test kits with brilliant, high-quality color cards for precise water analysis within minutes

> **Page 122**

0.002 mg/L – 1,500 mg/L



MQuant™ test strips

www.merckmillipore.com/test-strips

Easy-to-use, portable test strips for semi-quantitative detection of ions and organic or inorganic substances in a variety of samples

> **Page 138**

0.005 mg/L – 3,000 mg/L



MColorpHast™ pH test strips

www.merckmillipore.com/pH-tests

High-quality pH test strips and papers for reliable measurement of a broad pH range in all media types – even turbid liquids

> **Page 148**

0 – 14 pH

10 mg/L 100 mg/L 1,000 mg/L 10,000 mg/L 100,000 mg/L

Concentration

Parameters from A-Z

Visual and instrumental test kits at a glance

Our rapid tests offer numerous options for determining the concentration of individual parameters.

Use the Parameters to find the most suitable test for your application.

- Select your preferred test parameter (arranged alphabetically)
- Find your desired measuring range, then choose the most suitable products for your work
- You can use the order numbers to purchase products directly
- For further information about individual products, please visit www.merckmillipore.com/test-kits



Visual and instrumental test kits

Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
A Absorbance	-0.300 – 3.000 A			Physical method	58
Acid Capacity Cell Test to pH 4.3	0.40 – 8.00 mmol/L	120	1.01758.0001	Cell test	58
(total alkalinity)	20 – 400 mg/L CaCO ₃				
ADMI Color measurement				Application	58
Alkalinity (total)	see also Acid capacity to pH 4.3			Cell test	58
Alkalinity Test	0.1 – 10 mmol/L	200	1.11109.0001	Titration with pipette	128
Aluminium Cell Test	0.02 – 0.50 mg/L Al	25	1.00594.0001	Cell test	58
Aluminium Test	0.020 – 1.20 mg/L Al	350	1.14825.0001	Reagent test	58
Aluminium Test	0.07 – 0.8 mg/L Al	185	1.14413.0001	Color-card comparator	128
Aluminium Test	0.1 – 6 mg/L Al	150	1.18386.0001	Disk comparator	128
Aluminium Test	10 – 250 mg/L Al	100	1.10015.0001	Test strip	144
Ammonia, free	0.000 – 3.0 mg/L NH ₃ -N 0.000 – 3.65 mg/L NH ₃			Application	58
Ammonium Cell Test	0.010 – 2.000 mg/L NH ₄ -N 0.01 – 2.58 mg/L NH ₄	25	1.14739.0001	Cell test	58
Ammonium Test	0.010 – 3.00 mg/L NH ₄ -N 0.013 – 3.86 mg/L NH ₄	250 500	1.14752.0002 1.14752.0001	Reagent test	58
Ammonium Test	0.025 – 0.4 mg/L NH ₄	70	1.14428.0002	Color-card comparator	128
Ammonium Test	0.05 – 0.8 mg/L NH ₄	100	1.14400.0001	Color-card comparator	128
Ammonium Test	0.2 – 5 mg/L NH ₄	50	1.08024.0001	Sliding comparator	128
Ammonium Test	0.2 – 7 mg/L NH ₄	50	1.16892.0001	Test strip	120
Ammonium Test	0.2 – 8 mg/L NH ₄	200	1.14423.0002	Color-card comparator	128
Ammonium Test	0.2 – 8 mg/L NH ₄	200	1.14750.0002	Disk comparator	128
Ammonium Cell Test	0.20 – 8.00 mg/L NH ₄ -N 0.26 – 10.30 mg/L NH ₄	25	1.14558.0001	Cell test	58
Ammonium Test	0.5 – 10 mg/L NH ₄	150	1.11117.0001	Color card	128
Ammonium Test in freshwater and seawater	0.5 – 10 mg/L NH ₄	50	1.14657.0001	Color card	128
Ammonium Cell Test	0.5 – 16.0 mg/L NH ₄ -N 0.6 – 20.6 mg/L NH ₄	25	1.14544.0001	Cell test	58
Ammonium Test	2.0 – 150 mg/L NH ₄ -N 2.6 – 193 mg/L NH ₄	100	1.00683.0001	Reagent test	58
Ammonium Cell Test	4.0 – 80.0 mg/L NH ₄ -N 5.2 – 103.0 mg/L NH ₄	25	1.14559.0001	Cell test	58
Ammonium Test	5.0 – 20.0 mg/L NH ₄	50	1.16899.0001	Test strip	120
Ammonium Test	10 – 400 mg/L NH ₄	100	1.10024.0001	Test strip	144
Ammonium Test	20 – 180 mg/L NH ₄	50	1.16977.0001	Test strip	120
Antimony	0.10 – 8.00 mg/L Sb			Application	58
AOX Cell Test	0.05 – 2.50 mg/L AOX	25	1.00675.0001	Cell test	58
Arsenic Test	0.001 – 0.100 mg/L As	30	1.01747.0001	Reagent test	60
Arsenic Test	0.005 – 0.5 mg/L As	100	1.17927.0001	Test strip	144
Arsenic Test	0.02 – 3 mg/L As	100	1.17917.0001	Test strip	144
Ascorbic Acid Test	25 – 450 mg/L Ascorbic Acid	50	1.16981.0001	Test strip	120
Ascorbic Acid Test RQeasy®	25 – 450 mg/L Ascorbic Acid	50	1.17963.0001	Test strip	120
Ascorbic Acid Test	50 – 2,000 mg/L Ascorbic Acid	100	1.10023.0001	Test strip	144
B BOD Cell Test	0.5 – 3,000 mg/L BOD	50	1.00687.0001	Cell test	60
Boron Test	0.050 – 0.800 mg/L B	60	1.14839.0001	Reagent test	60

Parameters B-C

Visual and instrumental test kits

Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
B Boron Cell Test	0.05 – 2.00 mg/L B	25	1.00826.0001	Cell test	60
Bromate	0.5 – 200.0 µg/L BrO ₃ 1.0 – 200.0 µg/L BrO ₃			Application	60
Bromine Test	0.020 – 10.00 mg/L Br ₂	200	1.00605.0001	Reagent test	60
C Cadmium Test	0.0020 – 0.500 mg/L Cd	55	1.01745.0001	Reagent test	60
Cadmium Cell Test	0.025 – 1.000 mg/L Cd	25	1.14834.0001	Cell test	60
Calcium Test	0.20 – 4.00 mg/L Ca	100	1.00049.0001	Reagent test	60
Calcium Test	2 – 200 mg/L Ca	200	1.11110.0001	Titration with pipette	128
Calcium Test	2.5 – 45.0 mg/L Ca	50	1.16993.0001	Test strip	120
Calcium Test	5 – 125 mg/L Ca	50	1.16125.0001	Test strip	120
Calcium Test	5 – 160 mg/L Ca 7 – 224 mg/L CaO 12 – 400 mg/L CaCO ₃ 1.0 – 15.0 mg/L Ca 1.4 – 21.0 mg/L CaO 2.5 – 37.5 mg/L CaCO ₃	100	1.14815.0001	Reagent test	60
Calcium Test	10 – 100 mg/L Ca	60	1.10083.0001	Test strip	144
Calcium Cell Test	10 – 250 mg/L Ca 14 – 350 mg/L CaO 25 – 624 mg/L CaCO ₃	25	1.00858.0001	Cell test	62
Carbohydrazide	see Oxygen Scavengers Test			Reagent test	62
Carbonate Hardness Test / Acid capacity to pH 4.3 ("SBV", ANC)	0.25 – 25 °e (ANC 0.1 – 7.2 mmol/L)	300	1.08048.0001	Titration with pipette	128
Carbonate Hardness Test / Acid capacity to pH 4.3 ("SBV", ANC)	1 drop corresponds to 1.25 °e	100	1.11103.0001	Titration with dropping bottle	128
Carbonate Hardness Test in freshwater and seawater	1 drop corresponds to 1.25 °e	50	1.14653.0001	Titration with dropping bottle	128
Carbonate Hardness Test	5 – 30 °e	100	1.10648.0001	Test strip	144
Carbon Dioxide Test	1.25 mg/L CO ₂ 2.5 mg/L CO ₂ 5 mg/L CO ₂	100	1.17179.0001	Titration with dropping bottle	128
Chloride Test	0.10 – 5.00 mg/L Cl	100	1.01807.0001	Reagent test	62
Chloride Cell Test	0.5 – 15.0 mg/L Cl	25	1.01804.0001	Cell test	62
Chloride Test	2 – 200 mg/L Cl	200	1.11106.0001	Titration with pipette	128
Chloride Test	2.5 – 250 mg/L Cl	100 175	1.14897.0001 1.14897.0002	Reagent test	62
Chloride Test	3 – 300 mg/L Cl	200	1.14753.0001	Disk comparator	128
Chloride Cell Test	5 – 125 mg/L Cl	25	1.14730.0001	Cell test	62
Chloride Test	5 – 300 mg/L Cl	400	1.14401.0001	Color-card comparator	128
Chloride Test	1 drop corresponds to 25 mg/L Cl	100	1.11132.0001	Titration with dropping bottle	128
Chloride Test	500 – 3,000 mg/L Cl	100	1.10079.0001	Test strip	144
Chlorine Test (free chlorine)	0.01 – 0.3 mg/L Cl ₂	400	1.14434.0001	Color-card comparator	128
Chlorine Test (free chlorine)	0.010 – 6.00 mg/L Cl ₂	200 1,200	1.00598.0002 1.00598.0001	Reagent test	62
Chlorine Cell Test (free chlorine)	0.03 – 6.00 mg/L Cl ₂	200	1.00595.0001	Cell test	62

Visual and instrumental test kits

Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
C Chlorine Test (free chlorine) in freshwater and seawater	0.1 – 2 mg/L Cl ₂	100	1.14670.0001	Color card	128
Chlorine Test (free chlorine) (liquid)	0.1 – 2 mg/L Cl ₂	600	1.14978.0001	Disk comparator	128
Chlorine Test (free chlorine)	0.25 – 15 mg/L Cl ₂	1000	1.14976.0001	Disk comparator	128
Chlorine Test (free chlorine)	0.5 – 10.0 mg/L Cl ₂	50	1.16896.0001	Test strip	120
Chlorine Test (free chlorine)	0.5 – 20 mg/L Cl ₂	75	1.17925.0001	Test strip	144
Chlorine Test (free chlorine)	25 – 500 mg/L Cl ₂	100	1.17924.0001	Test strip	144
Chlorine Test (total chlorine)	0.010 – 6.00 mg/L Cl ₂	200	1.00602.0001	Reagent test	62
		1200	1.00602.0002		
Chlorine Test (free and total chlorine)	0.010 – 6.00 mg/L Cl ₂	200 (100 each)	1.00599.0001	Reagent test	62
Chlorine Cell Test (free and total chlorine)	0.03 – 6.00 mg/L Cl ₂	200 (100 each)	1.00597.0001	Cell test	62
Chlorine Test (liquid) (free and total chlorine)	0.1 – 2 mg/L Cl ₂	800 (400 each)	1.14801.0001	Disk comparator	128
Chlorine Test (free and total chlorine)	0.25 – 15 mg/L Cl ₂	800 (400 each)	1.14826.0001	Disk comparator	130
Chlorine Reagent Cl ₂ -1 (liquid)	0.010 – 6.00 mg/L Cl ₂	200	1.00086.0001	Reagent test	62
Chlorine Reagent Cl ₂ -2 (liquid)	0.010 – 6.00 mg/L Cl ₂	400	1.00087.0001	Reagent test	62
Chlorine Reagent Cl ₂ -3 (liquid)	0.010 – 6.00 mg/L Cl ₂	600	1.00088.0001	Reagent test	62
Chlorine- and pH Test (free chlorine)	0.1 – 1.5 mg/L Cl ₂ pH 6.5 – 7.9	150 (chlorine) 150 (pH)	1.11160.0001	Sliding comparator	130
Chlorine- and pH Test (free and total chlorine)	0.1 – 1.5 mg/L Cl ₂ pH 6.8 – 7.8	200 (chlorine) 200 (pH)	1.11174.0001	Color-matching vessel	130
Chlorine Dioxide Test	0.020 – 0.55 mg/L ClO ₂	300	1.18754.0001	Color-card comparator	130
Chlorine Dioxide Test	0.020 – 10.00 mg/L ClO ₂	200	1.00608.0001	Reagent test	62
Chlorine Dioxide Test	0.50 – 28 mg/L ClO ₂	300	1.18756.0001	Disk comparator	130
Chlorophyll-a and phaeophytin-a				Application	62
Chlorophyll-a, -b, -c				Application	62
Chromate Test for the determination of chromium (VI)	0.010 – 3.00 mg/L Cr 0.02 – 6.69 mg/L CrO ₄	250	1.14758.0001	Reagent test	64
Chromate Cell Test for the determination of chromium (VI) and chromium (total)	0.05 – 2.00 mg/L Cr 0.11 – 4.46 mg/L CrO ₄	25	1.14552.0001	Cell test	64
Chromate Test	0.01 – 0.22 mg/L CrO ₄	150	1.14402.0001	Color-card comparator	130
Chromate Test	0.2 – 3.6 mg/L CrO ₄	300	1.14441.0001	Color-card comparator	130
Chromate Test	0.2 – 22 mg/L CrO ₄	300	1.14756.0001	Disk comparator	130
Chromate Test	3 – 100 mg/L CrO ₄	100	1.10012.0001	Test strip	144
Chromium in electroplating baths	4 – 400 g/L CrO ₃			Application	64
Cobalt Test	10 – 1,000 mg/L Co	100	1.10002.0001	Test strip	144
COD Cell Test	4.0 – 40.0 mg/L COD	25	1.14560.0001	Cell test	64
COD Cell Test	5.0 – 80.0 mg/L COD		1.01796.0001	Cell test	64
COD Cell Test	10 – 150 mg/L COD	25	1.14540.0001	Cell test	64
COD Cell Test	15 – 300 mg/L COD	25	1.14895.0001	Cell test	64
COD Cell Test	25 – 1,500 mg/L COD	25	1.14541.0001	Cell test	64
COD Cell Test	50 – 500 mg/L COD	25	1.14690.0001	Cell test	64
COD Cell Test	300 – 3,500 mg/L COD	25	1.14691.0001	Cell test	64

Parameters C-F

Visual and instrumental test kits

Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
C COD Cell Test	500 – 10,000 mg/L COD	25	1.14555.0001	Cell test	64
COD Cell Test	5000 – 90,000 mg/L COD	25	1.01797.0001	Cell test	64
COD Cell Test for seawater / high chloride contents	5.0 – 60.0 mg/L COD	25	1.17058.0001	Cell test	64
COD Cell Test for seawater / high chloride contents	50 – 3,000 mg/L COD	25	1.17059.0001	Cell test	64
COD Cell Test (Hg free)	10 – 150 mg/L COD	25	1.09772.0001	Cell test	66
COD Cell Test (Hg free)	100 – 1,500 mg/L COD	25	1.09773.0001	Cell test	66
Color, ADMI				Physical method	66
Color, Hazen				Physical method	66
Color, Hazen				Physical method	66
Color, Spectral Absorption Coefficient				Physical method	66
Color, true color				Physical method	66
Color Test	5 – 150 Hz	no limit	1.14421.0001	Color-card comparator	130
Compact Laboratory for water testing			1.11151.0001	Compact lab	137
Congo red paper	pH <3 blue-violet / >5 red-orange	3 x 4.8 m	1.09514.0003	pH test paper	152
Copper Test	0.02 – 6.00 mg/L Cu	250	1.14767.0001	Reagent test	66
Copper Test	0.05 – 0.5 mg/L Cu	125	1.14414.0001	Color-card comparator	130
Copper Cell Test	0.05 – 8.00 mg/L Cu	25	1.14553.0001	Cell test	66
Copper Test in freshwater and seawater	0.15 – 1.6 mg/L Cu	50	1.14651.0001	Color card	130
Copper Test	0.3 – 5 mg/L Cu	125	1.14418.0001	Color-card comparator	130
Copper Test	0.3 – 10 mg/L Cu	125	1.14765.0001	Disk comparator	130
Copper Test	10 – 300 mg/L Cu	100	1.10003.0001	Test strip	144
Copper in electroplating baths	2.0 – 80.0 g/L Cu			Application	66
Cyanide Test	0.002 – 0.03 mg/L CN	65	1.14417.0001	Color-card comparator	130
Cyanide Test for the determination of free and readily liberated cyanide	0.0020 – 0.500 mg/L CN	100	1.09701.0001	Reagent test	66
Cyanide Cell Test	0.010 – 350 µg/L CN	25	1.02531.0001	Cell test	66
Cyanide Cell Test for the determination of free and readily liberated cyanide	0.010 – 0.500 mg/L CN	25	1.14561.0001	Cell test	66
Cyanide Test	0.03 – 0.7 mg/L CN	200	1.14429.0001	Color-card comparator	130
Cyanide Test	0.03 – 5 mg/L CN	200	1.14798.0001	Disk comparator	130
Cyanide Test	1 – 30 mg/L CN	100	1.10044.0001	Test strip	144
Cyanuric acid Test	2 – 160 mg/L Cyanuric acid	100	1.19253.0001	Reagent test	66
D DEHA (Diethylhydroxylamine)	see Oxygen Scavengers Test			Reagent test	68
Detergents	see Surfactants			Cell test	68
F Fluoride Test	0.02 – 2.00 mg/L F	250 mL	1.00822.0250	Reagent test	68
Fluoride Cell Test	0.10 – 1.80 mg/L F	25	1.00809.0001	Cell test	68
	0.025 – 0.500 mg/L F				
Fluoride Test	0.10 – 20.0 mg/L F	100	1.14598.0001	Reagent test	68
		250	1.14598.0002		
Fluoride Test	0.15 – 0.8 mg/L F	100	1.18771.0001	Color card	130
Formaldehyde Test	0.02 – 8.00 mg/L HCHO	100	1.14678.0001	Reagent test	68
Formaldehyde Test	0.1 – 1.5 mg/L HCHO	100	1.08028.0001	Sliding comparator	130

Visual and instrumental test kits

Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
F Formaldehyde Cell Test	0.10 – 8.00 mg/L HCHO	25	1.14500.0001	Cell test	68
Formaldehyde Test	1.0 – 45.0 mg/L HCHO	50	1.16989.0001	Test strip	120
Formaldehyde Test	10 – 100 mg/L HCHO	100	1.10036.0001	Test strip	144
Free Fatty Acids	0.5 – 3.0 mg/g KOH	100	1.17046.0001	Test strip	144
G Glucose Test	1 – 100 mg/L Glucose	50	1.16720.0001	Test strip	120
Glucose Test	10 – 500 mg/L Glucose	50	1.17866.0001	Test strip	144
Gold Test	0.5 – 12.0 mg/L Au	75	1.14821.0002	Reagent test	68
H Hardness	see Residual Hardness or Total Hardness			Color card	134
Hazen Color Number (Pt/Co, APHA, Hazen)	0 – 1,000 Pt/Co or Cu			Physical method	68
Hydrazine Test	0.005 – 2.00 mg/L N ₂ H ₄	100	1.09711.0001	Reagent test	68
Hydrazine Test	0.1 – 1 mg/L N ₂ H ₄	100	1.08017.0001	Color-matching vessel	130
Hydrogen Peroxide	see also Peroxide			Test strip	120
Hydrogen Peroxide Test	0.015 – 6.00 mg/L H ₂ O ₂	100	1.18789.0001	Reagent test	68
Hydrogen Peroxide Cell Test	2.0 – 20.0 mg/L H ₂ O ₂	25	1.14731.0001	Cell test	68
	0.25 – 5.00 mg/L H ₂ O ₂				
Hydrogen sulfide	see Sulfide			Reagent test	68
Hydroquinone	see Oxygen Scavengers Test			Reagent test	68
Hydroxymethylfurfural Test	1.0 – 60.0 mg/L HMF	50	1.17952.0001	Test strip	120
I Iodine Color Number	0.010 – 50.0 IFZ			Physical method	68
Iodine Test	0.050 – 10.00 mg/L I ₂	200	1.00606.0001	Reagent test	68
Iron Test	0.0025 – 5.00 mg/L Fe	250	1.14761.0002	Reagent test	68
		1,000	1.14761.0001		
Iron Test	0.01 – 0.2 mg/L Fe	300	1.14403.0001	Color-card comparator	130
Iron Test	0.010 – 5.00 mg/L Fe	150	1.00796.0001	Reagent test	68
Iron Test in freshwater and seawater	0.05 – 1 mg/L Fe	50	1.14660.0001	Color card	130
Iron Cell Test	0.05 – 4.00 mg/L Fe	25	1.14549.0001	Cell test	68
Iron Test	0.1 – 5 mg/L Fe	500	1.14759.0001	Disk comparator	130
Iron Test	0.1 – 50 mg/L Fe	200	1.11136.0001	Color-matching vessel	130
Iron Test	0.2 – 2.5 mg/L Fe	500	1.14438.0001	Color-card comparator	130
Iron Test	0.25 – 15 mg/L Fe	300	1.14404.0001	Color-card comparator	132
Iron Test	0.5 – 20.0 mg/L Fe(II)	50	1.16982.0001	Test strip	120
Iron Cell Test	1.0 – 50.0 mg/L Fe	25	1.14896.0001	Cell test	68
Iron Test	3 – 500 mg/L Fe(II)	100	1.10004.0001	Test strip	144
Iron Test	20 – 200 mg/L Fe(II)	50	1.16983.0001	Test strip	120
Isoascorbic acid (Erythorbic acid)	see Oxygen Scavengers Test			Reagent test	68
L Lactic Acid Test	3 – 60.0 mg/L Lactic acid	50	1.16127.0001	Test strip	120
Lead Test	0.010 – 5.00 mg/L Pb	50	1.09717.0001	Reagent test	68
Lead Cell Test	0.10 – 5.00 mg/L Pb	25	1.14833.0001	Cell test	68
Lead Test	20 – 500 mg/L Pb	100	1.10077.0001	Test strip	144
Lead(II) acetat paper	Sulfide from 10 mg/L	3 x 4.8 m	1.09511.0003	Reagent paper	146
Litmus paper, blue	pH <7 red / >7 blue	3 x 4.8 m	1.09486.0003	pH test paper	152
Litmus paper, red	pH <7 red / >7 blue	3 x 4.8 m	1.09489.0003	pH test paper	152
M Magnesium Cell Test	5.0 – 75.0 mg/L Mg	25	1.00815.0001	Cell test	70
Magnesium Test	5 – 100 mg/L Mg	50	1.16124.0001	Test strip	120
Magnesium Test	100 – 1,500 mg/L Mg	50	1.11131.0001	Color card	132
Malic Acid Test	5.0 – 60.0 mg/L Malic acid	50	1.16128.0001	Test strip	120

Parameters M-N

Visual and instrumental test kits

	Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
M	Manganese Test	0.005 – 2.00 mg/L Mn	250	1.01846.0001	Reagent test	70
	Manganese Test	0.010 – 10.0 mg/L Mn	250	1.14770.0002	Reagent test	70
			500	1.14770.0001		
	Manganese Test	0.03 – 0.5 mg/L Mn	120	1.14406.0001	Color-card comparator	132
	Manganese Cell Test	0.10 – 5.00 mg/L Mn	25	1.00816.0001	Cell test	70
	Manganese Test	0.3 – 10 mg/L Mn	120	1.14768.0001	Disk comparator	132
	Manganese Test	2 – 100 mg/L Mn	100	1.10080.0001	Test strip	144
	Mercury	0.025 – 1.000 mg/L Hg			Application	70
	Methylethylketoxime (2-Butanoneoxime)	see Oxygen Scavengers Test			Reagent test	70
	Molybdenum Cell Test	0.02 – 1.00 mg/L Mo 0.03 – 1.67 mg/L MoO ₄ ²⁺ 0.04 – 2.15 mg/L Na ₂ MoO ₄	25	1.00860.0001	Cell test	70
	Molybdenum Test	5 – 250 mg/L Mo	100	1.10049.0001	Test strip	144
	Monochloramine Test	0.050 – 10.00 mg/L Cl ₂ 0.036 – 7.26 mg/L NH ₂ Cl 0.010 – 1.98 mg/L NH ₂ Cl-N	150	1.01632.0001	Reagent test	70
N	Nickel Test	0.02 – 0.5 mg/L Ni	125	1.14420.0001	Color-card comparator	132
	Nickel Test	0.02 – 5.00 mg/L Ni	250	1.14785.0001	Reagent test	70
	Nickel Cell Test	0.10 – 6.00 mg/L Ni	25	1.14554.0001	Cell test	70
	Nickel Test	0.5 – 10 mg/L Ni	500	1.14783.0001	Disk comparator	132
	Nickel Test	10 – 500 mg/L Ni	100	1.10006.0001	Test strip	144
	Nickel in electroplating baths	2.0 – 120 g/L Ni			Application	70
	Nitrate (UV)	0.0 – 7.0 mg/L			Application	70
	Nitrate Test	0.10 – 25.0 mg/L NO ₃ -N 0.4 – 110.7 mg/L NO ₃	100	1.09713.0001	Reagent test	70
			250	1.09713.0002		
	Nitrate Test	0.2 – 20.0 mg/L NO ₃ -N 0.9 – 88.5 mg/L NO ₃	100	1.14773.0001	Reagent test	70
	Nitrate Test	0.3 – 30.0 mg/L 1.3 – 132.8 mg/L	100	1.01842.0001	Reagent test	70
	Nitrate Cell Test	0.5 – 18.0 mg/L NO ₃ -N 2.2 – 79.7 mg/L NO ₃	25	1.14542.0001	Cell test	70
	Nitrate Cell Test	0.5 – 25.0 mg/L NO ₃ -N 2.2 – 110.7 mg/L NO ₃	25	1.14563.0001	Cell test	70
	Nitrate Test	3 – 90 mg/L NO ₃	50	1.16995.0001	Test strip	120
	Nitrate Cell Test	1.0 – 50.0 mg/L NO ₃ -N 4 – 221 mg/L NO ₃	25	1.14764.0001	Cell test	70
	Nitrate Test	5 – 90 mg/L NO ₃	90	1.18387.0001	Disk comparator	132
	Nitrate Test	5 – 225 mg/L NO ₃	50	1.16971.0001	Test strip	120
	Nitrate Test RQeasy®	5 – 250 mg/L NO ₃	50	1.17961.0001	Test strip	120
	Nitrate Test	10 – 150 mg/L NO ₃	200	1.11170.0001	Sliding comparator	132
	Nitrate Test	10 – 500 mg/L NO ₃	25	1.10020.0002	Test strip	144
			100	1.10020.0001		
	Nitrate Test	10 – 500 mg/L NO ₃	1,000	1.10092.0021	Individually sealed	144
	Nitrate Cell Test	23 – 225 mg/L NO ₃ -N 102 – 996 mg/L NO ₃	25	1.00614.0001	Cell test	70

Visual and instrumental test kits

Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
N Nitrate Cell Test in seawater	0.10 – 3.00 mg/L NO ₃ -N 0.4 – 13.3 mg/L NO ₃	25	1.14556.0001	Cell test	72
Nitrate Test in seawater	0.2 – 17.0 mg/L NO ₃ -N 0.9 – 75.3 mg/L NO ₃	50	1.14942.0001	Reagent test	72
Nitrate Test in freshwater	10 – 150 mg/L NO ₃	100	1.11169.0001	Color card	132
Nitrite Test	0.005 – 0.1 mg/L NO ₂	110	1.14408.0001	Color-card comparator	132
Nitrite Test	0.002 – 1.00 mg/L NO ₂ -N 0.007 – 3.28 mg/L NO ₂	335 1,000	1.14776.0002 1.14776.0001	Reagent test	72
Nitrite Test	0.025 – 0.5 mg/L NO ₂	200	1.08025.0001	Sliding comparator	132
Nitrite Cell Test	0.010 – 0.700 mg/L NO ₂ -N 0.03 – 2.30 mg/L NO ₂	25	1.14547.0001	Cell test	72
Nitrite Test	0.1 – 2 mg/L NO ₂	400	1.14424.0001	Color-card comparator	132
Nitrite Test	0.1 – 10 mg/L NO ₂	400	1.14774.0001	Disk comparator	132
Nitrite Test	0.5 – 10 mg/L NO ₂	75	1.10057.0001	Test strip	144
Nitrite Test	0.5 – 25.0 mg/L NO ₂	50	1.16973.0001	Test strip	120
Nitrite Test	2 – 80 mg/L NO ₂	25 100	1.10007.0002 1.10007.0001	Test strip	144
Nitrite Test in freshwater and seawater	0.05 – 1.0 mg/L NO ₂	100	1.14658.0001	Color card	132
Nitrite Cell Test	1.0 – 90.0 mg/L NO ₂ -N 3.3 – 295.2 mg/L NO ₂	25	1.00609.0001	Cell test	72
Nitrite Test	0.03 – 1.00 g/L NO ₂	50	1.16732.0001	Test strip	120
Nitrite Test	0.1 – 3 g/L NO ₂	100	1.10022.0001	Test strip	144
Nitrogen (total) Cell Test	0.5 – 15.0 mg/L N	25	1.00613.0001	Cell test	72
Nitrogen (total) Cell Test	0.5 – 15.0 mg/L N	25	1.14537.0001	Cell test	72
Nitrogen (total) Cell Test	10 – 150 mg/L N	25	1.14763.0001	Cell test	72
O Organic Carbon, Total	see TOC			Cell test	78
Oxifrit-Test®		60	1.10653.0001	Deep-frying fats test	136
Oxygen Test	0.1 – 10 mg/L O ₂	100	1.11107.0001	Titration with pipette	132
Oxygen Cell Test	0.5 – 12 mg/L O ₂	25	1.14694.0001	Cell test	72
Oxygen Test in freshwater and seawater	1 – 12 mg/L O ₂	50	1.14662.0001	Color card	132
Oxygen demand, biochemical	see BOD			Cell test	60
Oxygen demand, chemical	see COD			Cell test	64
Oxygen Scavengers Test	0.020 – 0.500 mg/L DEHA 0.027 – 0.666 mg/L Carbohy 0.05 – 1.32 mg/L Hydro 0.08 – 1.95 mg/L ISA 0.09 – 2.17 mg/L MEKO	200	1.19251.0001	Reagent test	72
Ozone Test	0.007 – 0.20 mg/L O ₃	300	1.18755.0001	Color-card comparator	132
Ozone Test	0.010 – 4.00 mg/L O ₃	200 1,200	1.00607.0001 1.00607.0002	Reagent test	72
Ozone Test	0.15 – 10 mg/L O ₃	300	1.18758.0001	Disk comparator	132

Parameters P

Visual and instrumental test kits

Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
P Palladium	0.05 – 1.25 mg/L Pd			Application	72
Peracetic Acid Test	1.0 – 22.5 mg/L Peracetic acid	50	1.16975.0001	Test strip	120
Peracetic Acid Test	5 – 50 mg/L Peracetic acid	100	1.10084.0001	Test strip	144
Peracetic Acid Test	20 – 100 mg/L Peracetic acid	50	1.17956.0001	Test strip	120
Peracetic Acid Test	75 – 400 mg/L Peracetic acid	50	1.16976.0001	Test strip	120
Peracetic Acid Test	100 – 500 mg/L Peracetic acid	100	1.10001.0001	Test strip	144
Peracetic Acid Test	500 – 2,000 mg/L Peracetic acid	100	1.17922.0001	Test strip	144
Peroxidase Test	yes/no result	100	1.17828.0001	Test strip	144
Peroxide	see also Hydrogen peroxide			Reagent test	68
Peroxide Test	0.2 – 20.0 mg/L H ₂ O ₂	50	1.16974.0001	Test strip	120
Peroxide Test	0.5 – 25 mg/L H ₂ O ₂	25	1.10011.0002	Test strip	146
		100	1.10011.0001		
Peroxide Test	1 – 100 mg/L H ₂ O ₂	100	1.10081.0001	Test strip	146
Peroxide Test	20.0 – 100 mg/L H ₂ O ₂	50	1.17968.0001	Test strip	120
Peroxide Test	100 – 1,000 mg/L H ₂ O ₂	50	1.16731.0001	Test strip	120
Peroxide Test	100 – 1,000 mg/L H ₂ O ₂	100	1.10337.0001	Test strip	146
pH indicator papers	see separate list of pH indicator papers	3 x 4.8 m		pH test paper	152
pH indicator strips	see separate list of pH indicator strips	100		pH test strips	153
pH Test	pH 1.0 – 5.0	50	1.16894.0001	Test strip	120
pH Test	pH 4.0 – 9.0	50	1.16996.0001	Test strip	120
pH Universal indicator liquid	pH 4 – 10	100 mL	1.09175.0100	Color card	132
		1 L	1.09175.1000		
pH Test	pH 4.5 – 9	100	1.08038.0001	Color-matching vessel	132
pH Test	pH 4.5 – 9	400	1.08027.0001	Sliding comparator	132
pH Test in freshwater and seawater	pH 5.0 – 9.0	200	1.18773.0001	Color-card comparator	132
pH Cell Test	pH 6.4 – 8.8	280	1.01744.0001	Cell test	72
pH Test in swimming pool	pH 6.5 – 8.2	200	1.14669.0001	Color card	134
pH Test for Cooling Lubricants	pH 7.0 – 10.0	50	1.16898.0001	Test strip	120
pH indicator liquid	pH 9 – 13	100 mL	1.09176.0100	Color card	132
Phaeophytin-a and Chlorophyll-a				Application	72
Phenol Test	0.002 – 0.100 mg/L Phenol 0.025 – 5.00 mg/L Phenol	50 – 250	1.00856.0001	Reagent test	72
Phenol Cell Test	0.10 – 2.50 mg/L Phenol	25	1.14551.0001	Cell test	72
Phenolphthalein paper	pH <8.5 colorless / >8.5 red	3 x 4.8 m	1.09521.0003	pH test paper	152
Phosphate Test (ortho-phosphate)	0.0025 – 5.00 mg/L PO ₄ -P 0.0077 – 15.30 mg/L PO ₄ 0.0057 – 11.46 mg/L P ₂ O ₅	220 420	1.14848.0002 1.14848.0001	Reagent test	72
Phosphate Test	0.046 – 0.43 mg/L PO ₄	200	1.18394.0001	Color-card comparator	134
Phosphate Test RQflex® plus	0.1 – 5.0 mg/L PO ₄	100	1.17942.0001	Reagent test	120
Phosphate Cell Test (ortho-phosphate)	0.05 – 5.0 mg/L PO ₄ -P 0.2 – 15.3 mg/L PO ₄ 0.11 – 11.46 mg/L P ₂ O ₅	25	1.00474.0001	Cell test	72
Phosphate Cell Test (ortho-phosphate and total phosphorus)	0.05 – 5.00 mg/L PO ₄ -P 0.2 – 15.3 mg/L PO ₄ 0.11 – 11.46 mg/L P ₂ O ₅	25	1.14543.0001	Cell test	74
Phosphate Test in freshwater and seawater	0.25 – 3 mg/L PO ₄	100	1.14661.0001	Color card	134

Visual and instrumental test kits

	Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
P	Phosphate Test	0.6 – 9.2 mg/L PO ₄	200	1.14846.0001	Disk comparator	134
	Phosphate Test	1.3 – 13.4 mg/L PO ₄	200	1.11138.0001	Color-matching vessel	134
	Phosphate Cell Test (ortho-phosphate)	0.5 – 25.0 mg/L PO ₄ -P	25	1.00475.0001	Cell test	74
		1.5 – 76.7 mg/L PO ₄				
		1.1 – 57.3 mg/L P ₂ O ₅				
	Phosphate Cell Test (ortho-phosphate and total phosphorus)	0.5 – 25.0 mg/L PO ₄ -P	25	1.14729.0001	Cell test	74
		1.5 – 76.7 mg/L PO ₄				
		1.1 – 57.3 mg/L P ₂ O ₅				
	Phosphate Cell Test (ortho-phosphate)	0.5 – 25.0 mg/L PO ₄ -P	25	1.14546.0001	Cell test	74
		1.5 – 76.7 mg/L PO ₄				
		1.1 – 57.3 mg/L P ₂ O ₅				
	Phosphate Test (ortho-phosphate)	0.5 – 30.0 mg/L PO ₄ -P	400	1.14842.0001	Reagent test	74
		1.5 – 92.0 mg/L PO ₄				
		1.1 – 68.7 mg/L P ₂ O ₅				
	Phosphate Test	3.1 – 123 mg/L PO ₄	190	1.14449.0001	Color-card comparator	134
	Phosphate Test (ortho-phosphate)	1.0 – 100.0 mg/L PO ₄ -P	100	1.00798.0001	Reagent test	74
		3 – 307 mg/L PO ₄				
		2 – 229 mg/L P ₂ O ₅				
	Phosphate Test	4.6 – 307 mg/L PO ₄	300	1.18388.0001	Disk comparator	134
	Phosphate Test	5 – 120 mg/L PO ₄	50	1.16978.0001	Test strip	120
	Phosphate Cell Test (ortho-phosphate)	3.0 – 100.0 mg/L PO ₄ -P	25	1.00616.0001	Cell test	74
		9 – 307 mg/L PO ₄				
		7 – 229 mg/L P ₂ O ₅				
Phosphate Cell Test (ortho-phosphate and total phosphorus)	3.0 – 100 mg/L PO ₄ -P	25	1.00673.0001	Cell test	74	
	9 – 307 mg/L PO ₄					
	7 – 229 mg/L P ₂ O ₅					
Phosphate Test	10 – 500 mg/L PO ₄	100	1.10428.0001	Test strip	146	
Platinum	0.10 – 1.25 mg/L Pt			Application	74	
Platinum-Cobalt Standard Method	see Color			Color-card comparator	130	
Potassium Test RQflex® plus	1.0 – 25.0 mg/L K	100	1.17945.0001	Reagent test	120	
Potassium Cell Test	5.0 – 50.0 mg/L K	25	1.14562.0001	Cell test	74	
Potassium Cell Test	30 – 300 mg/L K	25	1.00615.0001	Cell test	74	
Potassium Test	0.25 – 1.20 g/L K	50	1.16992.0001	Test strip	120	
Potassium Test	250 – 1,500 mg/L K	100	1.17985.0001	Test strip	146	
Potassium iodide-starch paper	Oxidizing agents	3 x 4.8 m	1.09512.0003	Reagent paper	146	
Protein-Test	0.01 – 1.4 g/L Protein	200	1.10306.0500	Reagent test	74	
Protein-Test	0.5 – 10 g/L Protein	250	1.10307.0500	Reagent test	74	
Q	Quaternary Ammonium Compounds	see also Surfactants (cationic)			Cell test	76
	Quaternary Ammonium Compounds	10 – 500 mg/L Benzalkonium chloride	100	1.17920.0001	Test strip	146
R	Residual Hardness Test	0.05 – 0.19 °e 0.7 – 2.7 mg/L CaCO ₃	400	1.11142.0001	Color card	134
	Residual Hardness Cell Test	0.50 – 5.00 mg/L Ca	25	1.14683.0001	Cell test	74
		0.070 – 0.700 °d				
		0.087 – 0.874 °e				
		0.12 – 1.25 °f				
		0.70 – 7.00 mg/L CaO				
		1.2 – 12.5 mg/L CaCO ₃				

Parameters S

Visual and instrumental test kits


Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
S SAC (Spectral absorption coefficient)	0.5 – 50.0 m ⁻¹			Physical method	74
Silicate (Silicic Acid) Test	0.0005 – 0.5000 mg/L SiO ₂ 0.00012 – 0.2337 mg/L Si	100	1.01813.0001	Reagent test	76
Silicate (Silicic Acid) Test	0.011 – 10.70 mg/L SiO ₂ 0.005 – 5.00 mg/L Si	300	1.14794.0001	Reagent test	76
Silicate (Silicic Acid) Test	0.01 – 0.25 mg/L Si 0.02 – 0.53 mg/L SiO ₂	150	1.14410.0001	Color-card comparator	134
Silicate (Silicic Acid) Test	0.3 – 10 mg/L Si 0.6 – 21 mg/L SiO ₂	150	1.14792.0001	Disk comparator	134
Silicate (Silicic Acid) Test	1.1 – 1,070 mg/L SiO ₂ 0.5 – 500 mg/L Si	100	1.00857.0001	Reagent test	76
Silicic Acid	see Silicate			Reagent test	76
Silver Test	0.25 – 3.00 mg/L Ag	100	1.14831.0001	Reagent test	76
Sodium Cell Test in nutrient solution for fertilization	10 – 300 mg/L Na	25	1.00885.0001	Cell test	76
Spectral Absorption Coefficient, Color	0.5 – 250 m ⁻¹			Application	76
Spectral Attenuation Coefficient	0.5 – 250 m ⁻¹			Application	76
Sucrose Test	0.25 – 2.5 g/L	50	1.16141.0001	Test strip	120
Sulfate Test	0.50 – 50.0 mg/L SO ₄	100	1.01812.0001	Reagent test	76
Sulfate Cell Test	5 – 250 mg/L SO ₄	25	1.14548.0001	Cell test	76
Sulfate Cell Test	5 – 300 mg/L SO ₄	100	1.02537.0001	Cell test	76
Sulfate Test	25 – 300 mg/L SO ₄	200	1.14791.0001	Cell test	76
Sulfate Test	25 – 300 mg/L SO ₄	75	1.18389.0001	Disk comparator	134
Sulfate Test	25 – 300 mg/L SO ₄	90	1.14411.0001	Color-card comparator	134
Sulfate Cell Test	50 – 500 mg/L SO ₄	25	1.00617.0001	Cell test	76
Sulfate Cell Test	100 – 1,000 mg/L SO ₄	25	1.14564.0001	Cell test	76
Sulfate Test	200 – 1,600 mg/L SO ₄	100	1.10019.0001	Test strip	146
Sulfide Test	0.02 – 0.25 mg/L S ²⁻	100	1.14416.0001	Color-card comparator	134
Sulfide Test	0.020 – 1.50 mg/L S ²⁻	220	1.14779.0001	Reagent test	73
Sulfide Test	0.1 – 5 mg/L S ²⁻	200	1.14777.0001	Disk comparator	134
Sulfite Test	0.5 – 50 mg/L Na ₂ SO ₃ (0.3 – 32 mg/L SO ₃)	200	1.11148.0001	Titration with pipette	134
Sulfite Cell Test	1.0 – 20.0 mg/L SO ₃ 0.05 – 3.00 mg/L SO ₃	25	1.14394.0001	Cell test	76
Sulfite Test	1.0 – 60.0 mg/L SO ₃ 0.8 – 48.0 mg/L SO ₂	150	1.01746.0001	Reagent test	76
Sulfite Test	10 – 200 mg/L SO ₃	50	1.16987.0001	Test strip	120
Sulfite Test	10 – 400 mg/L SO ₃	100	1.10013.0001	Test strip	146
Surfactants (anionic) Cell Test	0.05 – 2.00 mg/L MBAS	25	1.02552.0001	Cell test	76
Surfactants (cationic) Cell Test	0.05 – 1.50 mg/L CTAB	25	1.01764.0001	Cell test	76
Surfactants (nonionic) Cell Test	0.10 – 7.50 mg/L Triton® X-100	25	1.01787.0001	Cell test	76
Suspended Solids	25 – 750 mg/L suspended solids			Physical method	76

Visual and instrumental test kits

Parameter	Measuring range	No. of tests	Ord. No.	System / Type	Page
T Tin Cell Test	0.10 – 2.50 mg/L Sn	25	1.14622.0001	Cell test	78
Tin Test	10 – 200 mg/L Sn	50	1.10028.0001	Test strip	146
TOC Cell Test	5.0 – 80.0 mg/L TOC	25	1.14878.0001	Cell test	78
TOC Cell Test	50 – 800 mg/L TOC	25	1.14879.0001	Cell test	78
Total Alkalinity	see Acid capacity to pH 4.3 or Alkalinity			Cell test	58
Total Hardness Test	0.13 – 7 °e (1 – 100 mg/L CaCO ₃)	300	1.08047.0001	Titration with pipette	134
Total Hardness Test	0.1 – 30.0 °d	50	1.16997.0001	Test strip	120
Total Hardness Test	0.25 – 25 °e (0.1 – 3.6 mmol/L)	300	1.08039.0001	Titration with pipette	134
Total Hardness Cell Test	5 – 215 mg/L Ca 0.7 – 30.1 °d 0.9 – 37.6 °e 1.2 – 53.7 °f 7 – 301 mg/L CaO 12 – 537 mg/L CaCO ₃	25	1.00961.0001	Cell test	78
Total Hardness Test	1 drop corresponds to 1.25 °e	100	1.11104.0001	Titration with dropping bottle	134
Total Hardness Test	1 drop corresponds to 20 mg/L CaCO ₃	200	1.08312.0001	Titration with dropping bottle	134
Total Hardness Test in freshwater	1 drop corresponds to 1.25 °e	50	1.14652.0001	Titration with dropping bottle	134
Total Hardness Test	4 – 26 °e	100	1.10025.0001	Test strip	146
Total Hardness Test	4 – 26 °e	1,000	1.10032.0001	Individually sealed	146
Total Hardness Test	4 – 26 °e	5,000	1.10029.0001	Test strip	146
Total Hardness Test	6 – 31 °e	100	1.10046.0001	Test strip	146
Total Hardness Test	6 – 31 °e	25,000	1.10047.0013	Individually sealed	146
Total Hardness Test	<1.5 – >2.5 mmol/L CaCO ₃	100	1.17934.0001	Test strip	146
Total Nitrogen	see Nitrogen (total)			Cell test	72
Total Sugar Test (glucose and fructose)	65 – 650 mg/L total sugar	50	1.16136.0001	Test strip	120
Transmission	0.0 – 100.0 % T			Physical method	78
Turbidity	1 – 100 FAU			Physical method	78
U Urea Test for swimming pools	0.3 – 8 mg/L Urea	100	1.14843.0001	Disk comparator	134
Urea Test in Milk Application	0.2 – 7.0 mg/L NH ₄	50	1.16892.0001	Test strip	120
V Volatile Organic Acids Cell Test	50 – 3,000 mg/L acetic acid	25	1.01749.0001	Cell test	78
Volatile Organic Acids Test	50 – 3,000 mg/L acetic acid	100	1.01809.0001	Reagent test	78
W Water Hardness	see Residual Hardness or Total Hardness			Color card	134
Z Zinc Cell Test	0.025 – 1.000 mg/L Zn	25	1.00861.0001	Cell test	78
Zinc Test	0.05 – 2.50 mg/L Zn	100	1.14832.0001	Reagent test	78
Zinc Test	0.1 – 5 mg/L Zn	120	1.14780.0001	Disk comparator	134
Zinc Test	0.1 – 5 mg/L Zn	120	1.14412.0001	Color-card comparator	134
Zinc Cell Test	0.20 – 5.00 mg/L Zn	25	1.14566.0001	Cell test	78
Zinc Test	4 – 50 mg/L Zn	100	1.17953.0001	Test strip	146



Cooling & boiler water workflow

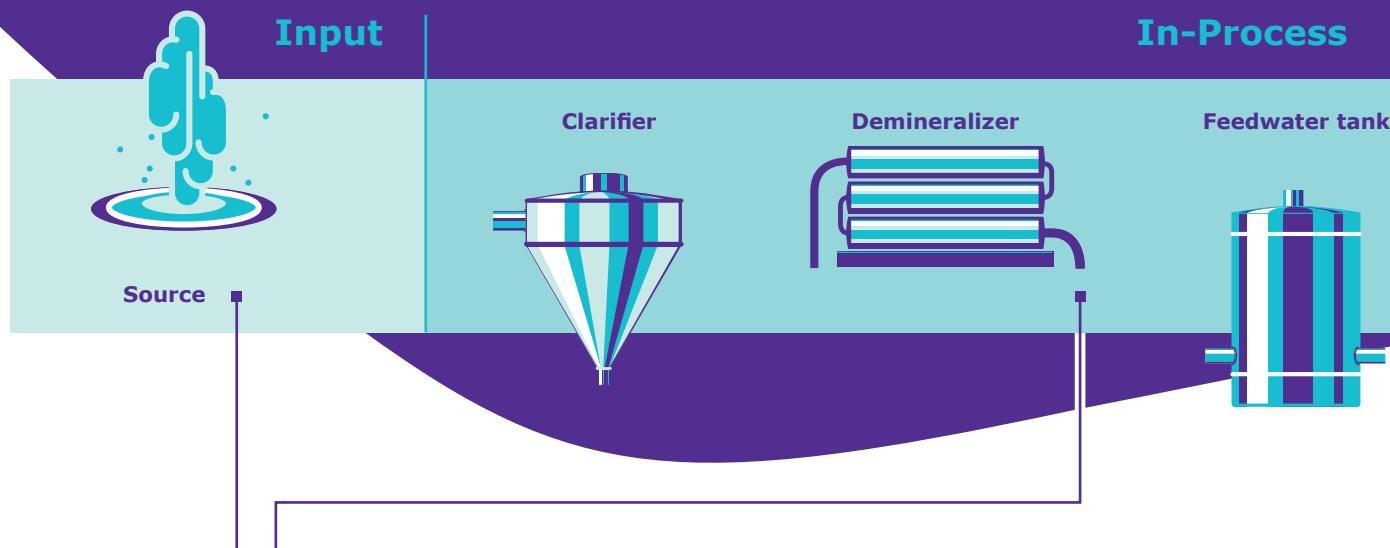

Quality Control


Sample Preparation

- Crack sets
> Page 51
- Syringe filters
> Page 163
- Thermoreactors, e.g. TR 620
> Page 52



Spectrophotometry

- Spectroquant® Prove 300/600
> Page 36
- Spectroquant® test kits, e.g. chloride, silicate, sulfate
> Page 54
- Sensitive measurements (100-mm cells)
> Page 54



Physical parameters

- Turbidimeter, e.g. Turbiquant® 3000
> Page 108
- Conductivity meters, pH meters
> Page 108

Microbial and pathogen testing

- Microbial filtration testing, e.g. EZ family
> Page 156
- Culture media, dehydrated and ready-to-use media
> Page 156



Water purification system

- Milli-Q® system
> Page 163




Reference materials

- CRM for test kits
> Page 102
- Certipur®
> Page 106
- CombiCheck
> Page 98



Analyzing cooling and boiler water is essential for power plants and industrial producers such as chemical, pharmaceutical, technical or food and beverage companies. Silicate, calcium and magnesium content is particularly important as they can cause deposit formation and scaling, leading to higher maintenance costs and downtimes.

The workflow diagram shows the products you need to test ultra-low levels of different parameters in process water. In particular, using Spectroquant® Prove 600 with a 100-mm cuvette allows ultra-sensitive measurements of silicate, chloride and iron to protect your system.

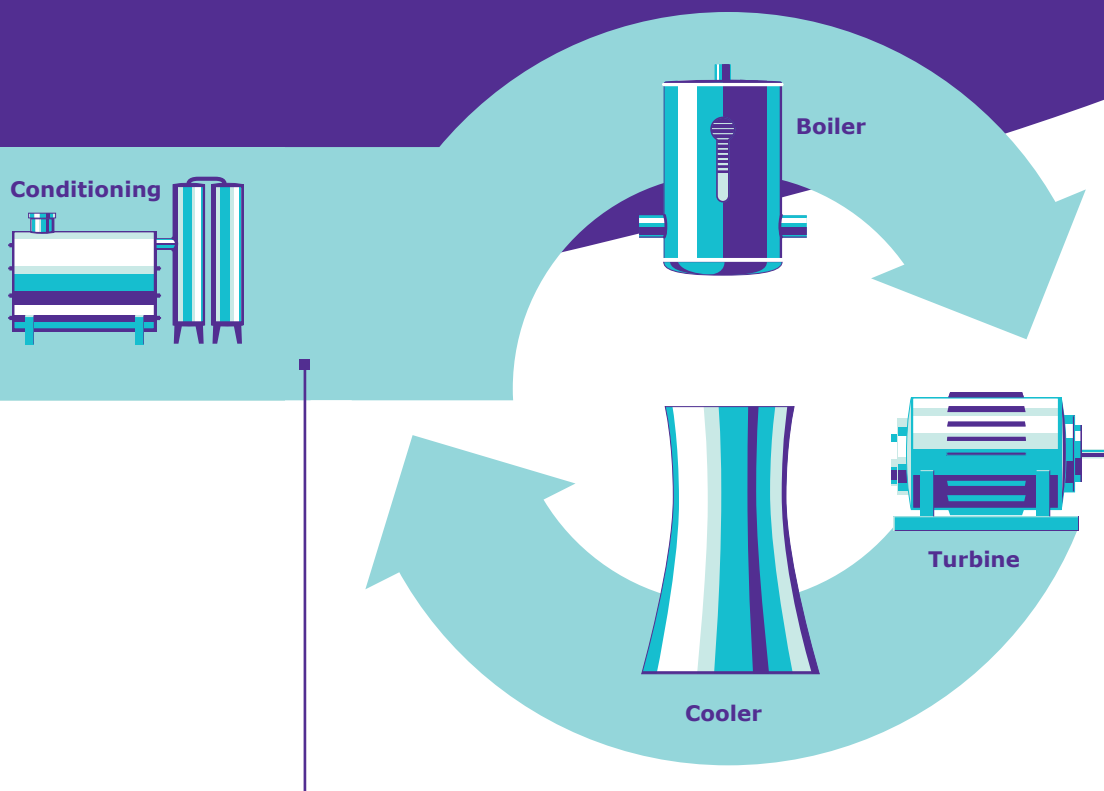

Mobile In-Process Control

Semi-quantitative testing

- pH strips and paper
> **Page 148**

- MQuant™ test strips,
e.g. chlorine
> **Page 138**

- MColortest™ test kits,
e.g. phosphate, iron
> **Page 122**



Quantitative testing

Photometry

- Move 100 and Move Cl₂/O₃/ClO₂/CyA/pH colorimeters
> **Page 40**

- Spectroquant® test kits,
e.g. silicate, chloride,
oxygen, sulfate
> **Page 54**



Microbial and pathogen testing

- Surface monitoring,
e.g. HY-LiTE®, HY-RiSE®
> **Page 157**

Physical parameters

- Turbidimeter,
e.g. Turbiquant® 1100
> **Page 108**




Reference materials

- CRM
> **Page 102**
- Certipur®
> **Page 106**



**MORE ABOUT
PHOSPHONATES**

in cooling and boiler water






wastewater workflow

Input



Wastewater supply

In-Process



Pre-sedimentation

Quality Control

Sample Preparation

- Crack Sets and Thermoreactors, e.g. TR 420
> **Page 50**
- Syringe filters
> **Page 163**
- Turbidimeter, e.g. Turbiquant® 1500
> **Page 108**
- Conductivity meters, pH meters
> **Page 108**



Spectrophotometry

- Spectroquant® Prove 100/300
> **Page 36**
- Spectroquant® test kits, e.g. BOD, COD, nitrogen
> **Page 54**



Microbial and pathogen testing

- Microbial filtration testing, e.g. EZ family
> **Page 156**
- Culture media, dehydrated and ready-to-use media
> **Page 156**



Water purification system

- Milli-Q® system
> **Page 163**




Reference materials

- CRM for test kits
> **Page 102**
- Certipur®
> **Page 106**
- CombiCheck
> **Page 98**



To protect the environment and communities, almost all governments require treatment and testing of municipal wastewater from households, and industrial wastewater from chemical, pharmaceutical, food, beverage and other production facilities.

The workflow diagram shows the products you need to analyze essential chemical parameters, such as COD, BOD, TOC, ammonium, nitrate, nitrite, total phosphorus and total nitrogen, as well as further important parameters like chromium, other heavy metals, and volatile organic acids (VOA).

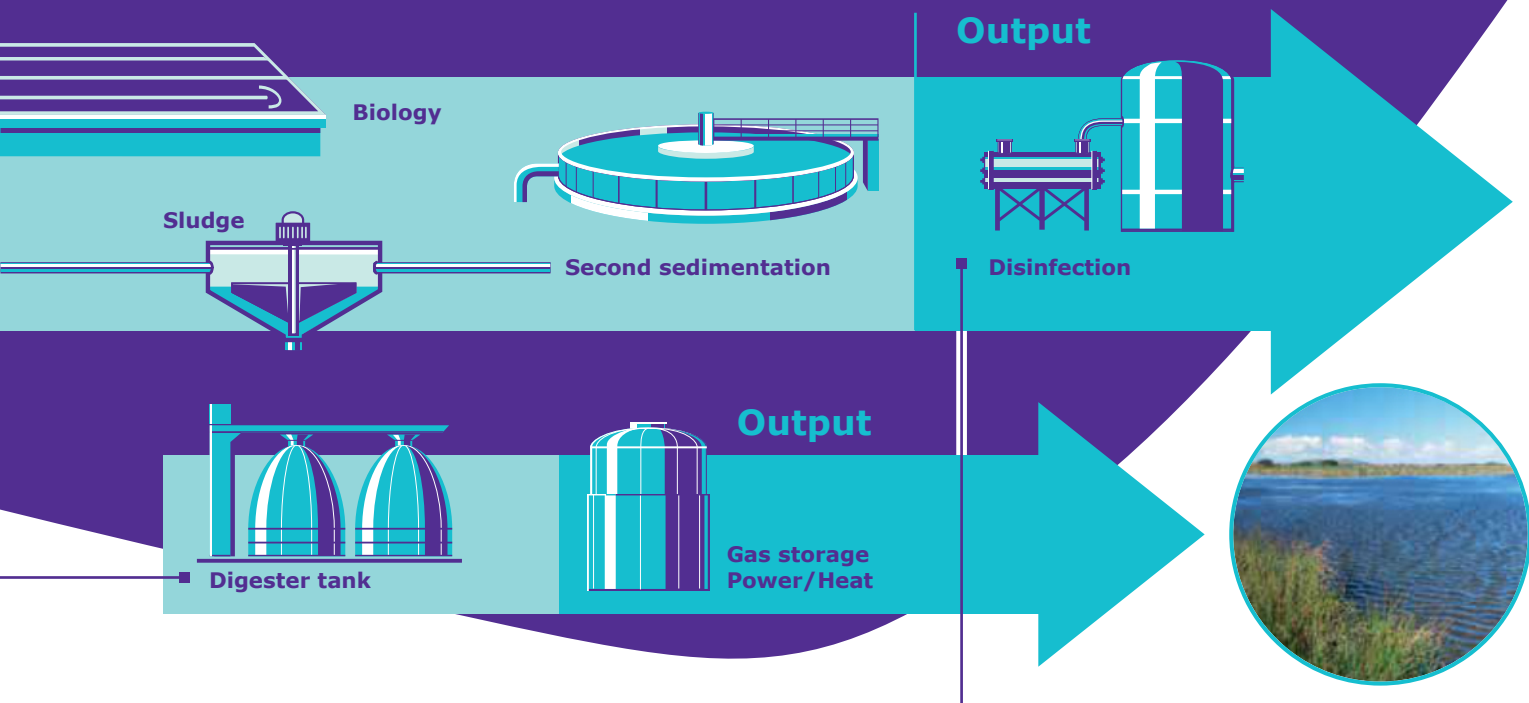

Mobile In-Process Control

Semi-quantitative testing

- pH strips and paper
> Page 148
- MQuant™ test strips,
e.g. chloride
> Page 138
- MColortest™ test kits,
e.g. phosphate, iron
> Page 122



Quantitative testing

Photometry

- Move 100 and Move $\text{Cl}_2/\text{O}_3/\text{ClO}_2/\text{CyA/pH}$ colorimeters
> Page 40
- Spectroquant® test kits,
e.g. chlorine,
phosphate, sulfate
> Page 54



Microbial and pathogen testing

- Air sampler,
e.g. MAS-family
> Page 157
- Surface monitoring,
e.g. HY-LITE®, HY-RiSE®
> Page 157



Physical parameters

- Turbidimeter, e.g. Turbiquant® 1100
> Page 108
- Conductivity meter, pH meter
> Page 108

Reference materials

- CRM
> Page 102
- Certipur®
> Page 106

**MORE ABOUT
SAMPLE
PREPARATION**




Learn more about
sample preparation

[www.merckmillipore.com/
webcast_asp_wfa_sampleprep](http://www.merckmillipore.com/webcast_asp_wfa_sampleprep)



drinking water workflow

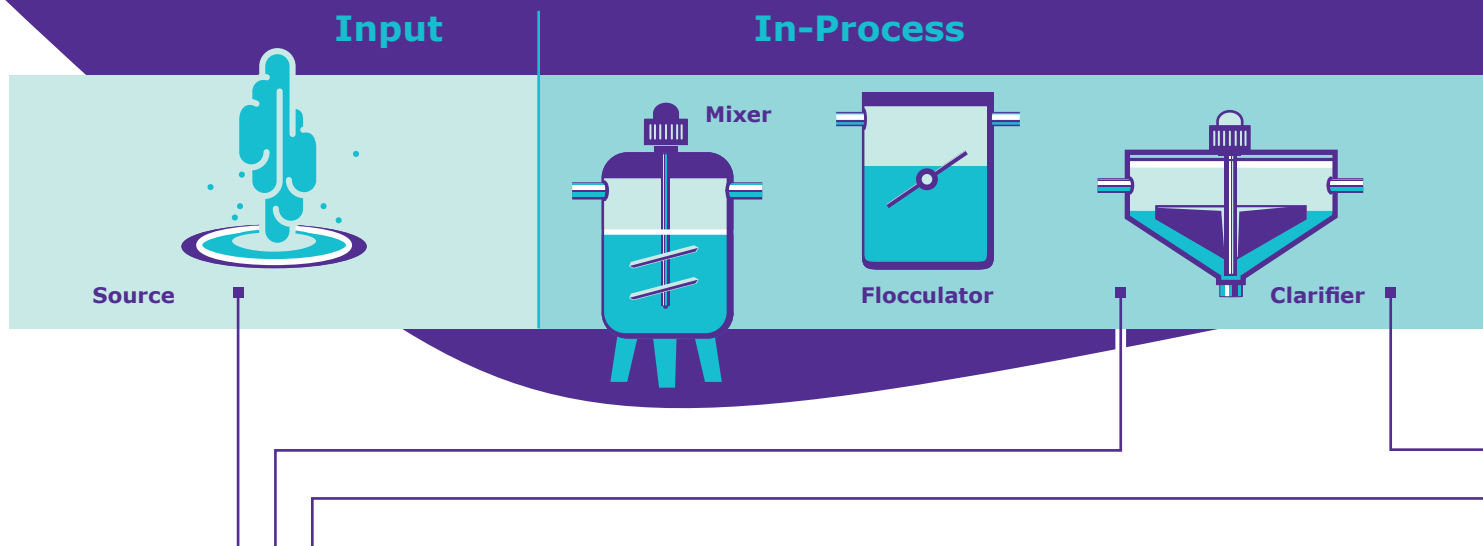

Quality Control

Chromatography

- HPLC, GC, TLC
> **Page 158**
- Syringe filters
> **Page 163**
- Solvents and inorganic reagents
> **Page 159**



Spectrophotometry

- Spectroquant® Prove 300/600
> **Page 36**
- Spectroquant® test kits, e.g. ammonium, fluoride, nitrate
> **Page 54**
- For sensitive measurements (100-mm cell)
> **Page 54**



Physical parameters

- Turbidimeter, e.g. Turbiquant® 3000
> **Page 108**
- Conductivity meter, pH meter
> **Page 108**

Microbial and pathogen testing

- Microbial filtration testing, e.g. EZ family
> **Page 156**
- Culture media, dehydrated and ready-to-use media
> **Page 156**



Water purification system

- Milli-Q® system
> **Page 163**



Reference materials


- CRM for test kits
> **Page 102**
- Certipur®
> **Page 106**
- Standards for pesticides
> **Page 160**



Learn more about workflow steps and products: www.just-prove-it.com
Find all the products you need: www.sigma-aldrich.com

Any industry that produces, uses, or processes drinking water must comply with national regulations and perform regular tests to ensure that drinking water is free of chemical and microbiological contaminations.

The workflow diagram shows the products you need to test important chemical parameters, such as aluminum, ammonium, bromate, iron, manganese, chloride, nitrate, nitrite, sulfate, chromium and other metals, or microbiological contamination.

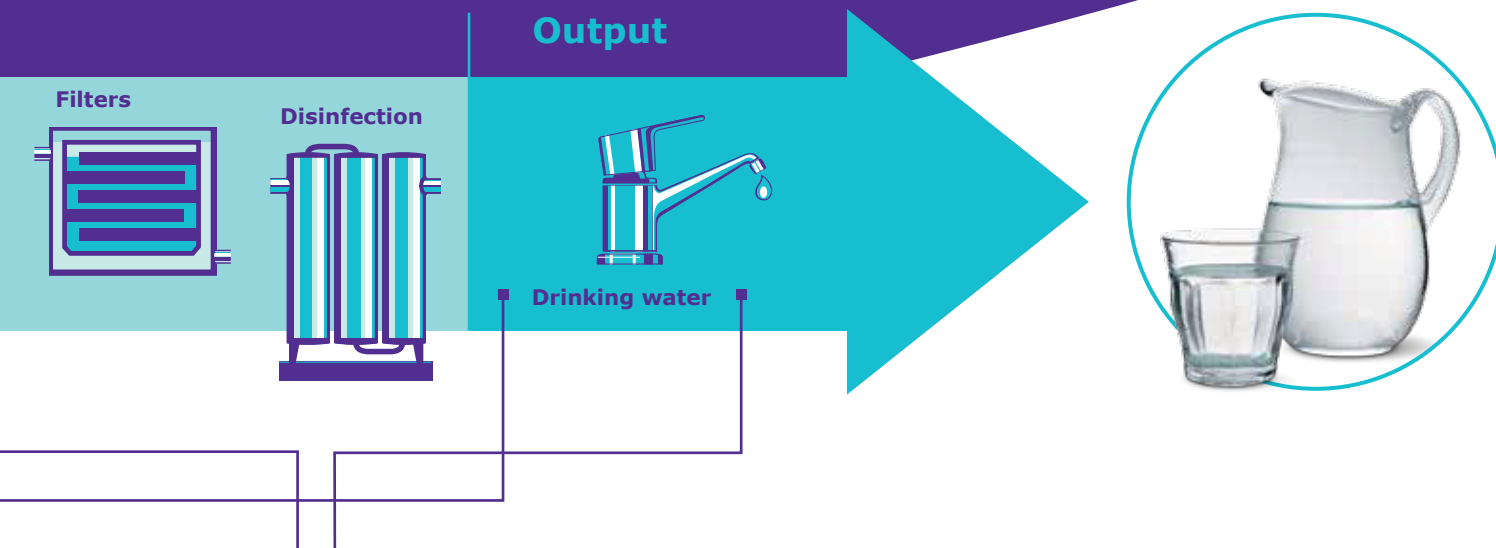

Mobile In-Process Control

Semi-quantitative testing

- pH strips and paper
> Page 148
- MQuant™ test strips,
e.g. peracetic acid
> Page 138



Quantitative testing

Photometry

- Move 100 and Move Cl₂/O₃/
ClO₂/CyA/pH colorimeters
> Page 40
- Spectroquant® test kits,
e.g. ozone, chlorine
> Page 54



Physical parameters

- Conductivity meter, pH meter
> Page 108



Microbial and pathogen testing

- Air sampler,
e.g. MAS-family
> Page 157
- Surface monitoring,
e.g. HY-LiTE®, HY-RiSE®
> Page 157



Reference materials

- CRM
> Page 102
- Certipur®
> Page 106




PARAMETERS FOR DRINKING WATER

Check the range of different parameters in the drinking water guidelines table on page 57



bottled water workflow

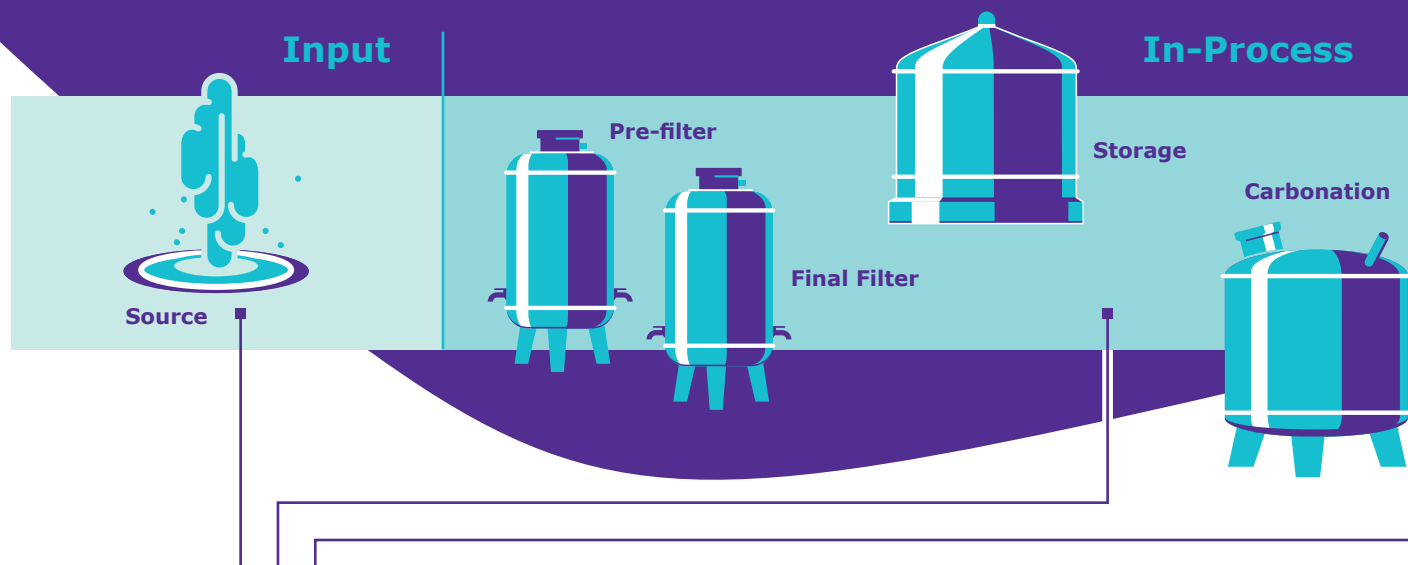

Quality Control

Chromatography

- HPLC, GC, TLC
> **Page 158**

- Syringe filters
> **Page 163**

- Inorganic reagents
> **Page 158**

Spectrophotometry

- Spectroquant® Prove 300/600
> **Page 36**

- Spectroquant® test kits, e.g. calcium, bromate
> **Page 54**

- For sensitive measurements (100-mm cell)
> **Page 54**

Physical parameters

- Turbidimeter, e.g. Turbiquant® 1500
> **Page 108**

Microbial and pathogen testing

- Microbial filtration testing, e.g. EZ family
> **Page 156**

- Culture media, dehydrated and ready-to-use media
> **Page 156**

Water purification system

- Milli-Q® system
> **Page 163**

Reference materials


- CRM for test kits
> **Page 102**

- Certipur®
> **Page 106**

- Standards for pesticides
> **Page 160**

One of the main challenges in processing and producing bottled water is consistently maintaining high product quality to protect consumers and the environment. To ensure this, the efficacy of flocculation and filtration should be tested through parameters such as aluminum, iron, manganese, calcium, fluoride and total hardness.

The workflow diagram shows the products you need for chemical and microbiological analysis of bottled water, including culture media, membranes, filter funnels, filtration devices, hardware, and accessories.

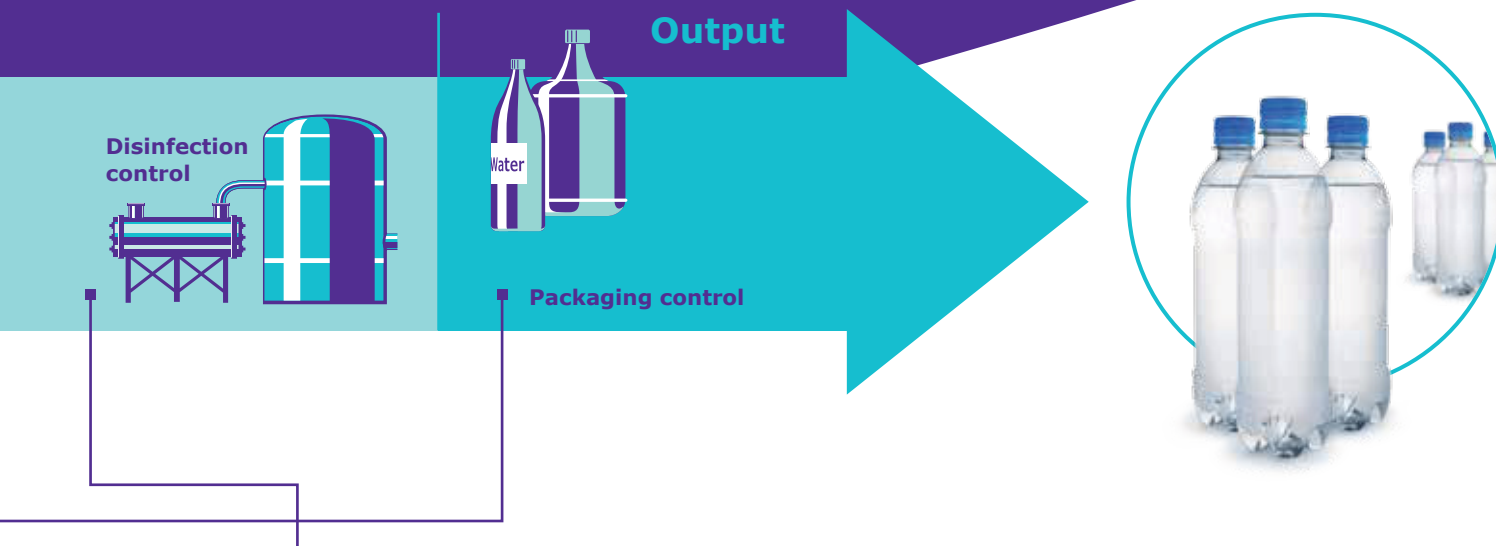

Mobile In-Process Control

Semi-quantitative testing

- pH strips and paper
> Page 148
- MQuant™ test strips,
e.g. chlorine, peracetic acid
> Page 138



Quantitative testing

Photometry

- Move 100 and Move Cl₂/O₃/
ClO₂/CyA/pH colorimeters
> Page 40
- Spectroquant® test kits,
e.g. ozone, chlorine
> Page 54



Test strips

- RQflex® 10
> Page 114
- Reflectoquant® disinfectant
parameter test kits, e.g. chlorine
> Page 120

Microbial and pathogen testing

- Air sampler,
e.g. MAS-family
> Page 157
- Surface monitoring,
e.g. HY-LITE®, HY-RISE®
> Page 157



Physical parameters

- Turbidimeter, e.g. Turbiquant® 1100
> Page 108
- Conductivity meter, pH meter
> Page 108

Reference materials

- CRM
> Page 102
- Certipur®
> Page 106




**MORE ABOUT
BROMATE
ANALYSIS**

For more information about bromate analysis of drinking water see page 32



Brewery workflow

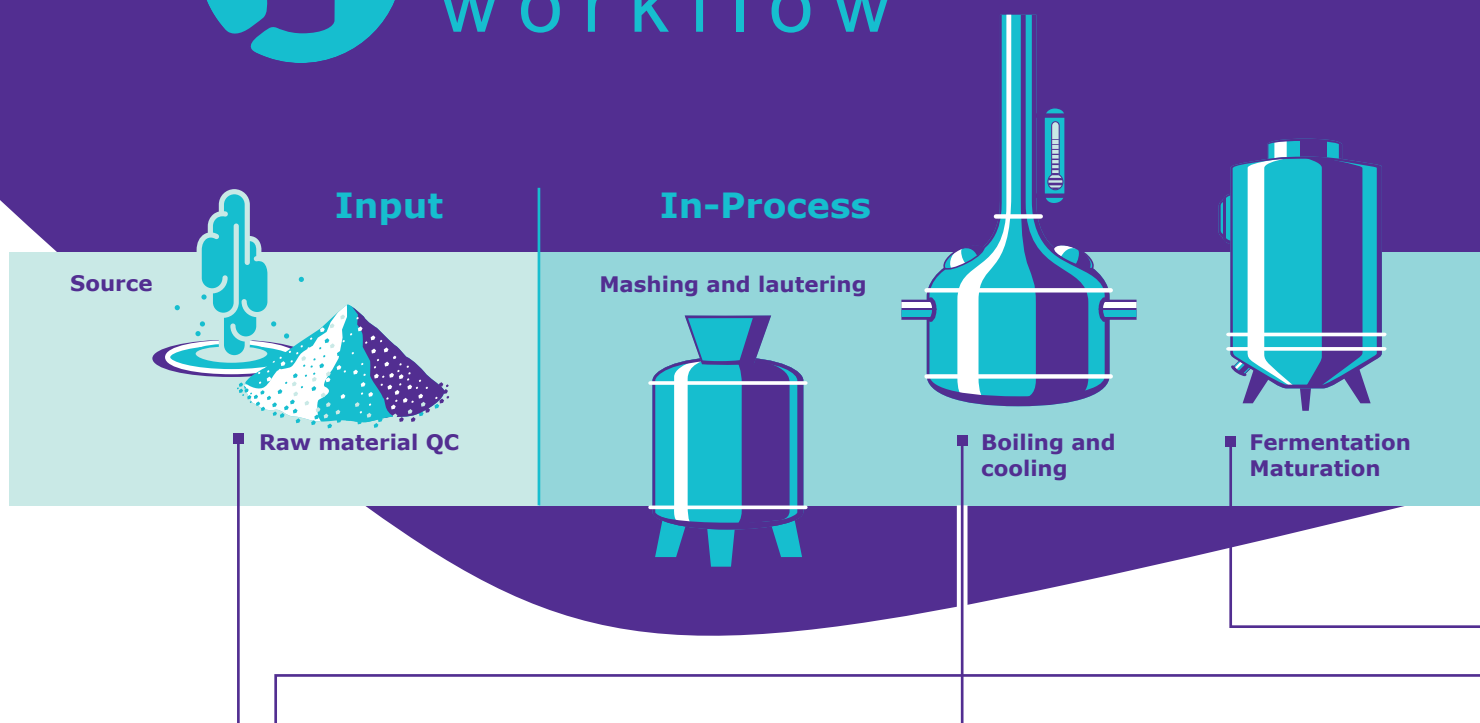

Quality Control

Chromatography

- HPLC, GC, TLC
> Page 158
- Syringe filters
> Page 163
- Solvents and inorganic reagents
> Page 159



Spectrophotometry

- Spectroquant® Prove 300
> Page 36
- Brewery methods acc. to international standards
> Page 46



Reference materials

- CRM for test kits
> Page 102
- Certipur®
> Page 106
- Standards for pesticides
> Page 160



Microbial and pathogen testing

- Microbial filtration testing, e.g. EZ family
> Page 156
- Culture media, dehydrated and ready-to-use media
> Page 156



Water purification system

- Milli-Q® system
> Page 163



Physical parameters

- Turbidimeter, e.g. Turbiquant® 3000
> Page 108
- pH-meters
> Page 108




Ingredient and nutritional testing

- Flavors and fragrances
> Page 161
- Karl Fischer - reagents
> Page 162

Breweries need to carefully monitor all stages of production – from analyzing raw materials and drinking water, to in-process and disinfection controls, and finally testing the finished product and wastewater (see “wastewater workflow” on page 22). Beer quality and consistency are judged through parameters such as bitterness, flavonoids, free amino nitrogen, color, calcium and zinc content, and microbiological contamination.

The workflow diagram shows the products you need for reliable beer analysis. In particular, Spectroquant® Prove spectrophotometers feature pre-programmed methods according to international standards to help you quickly and accurately monitor beer quality and maturity.

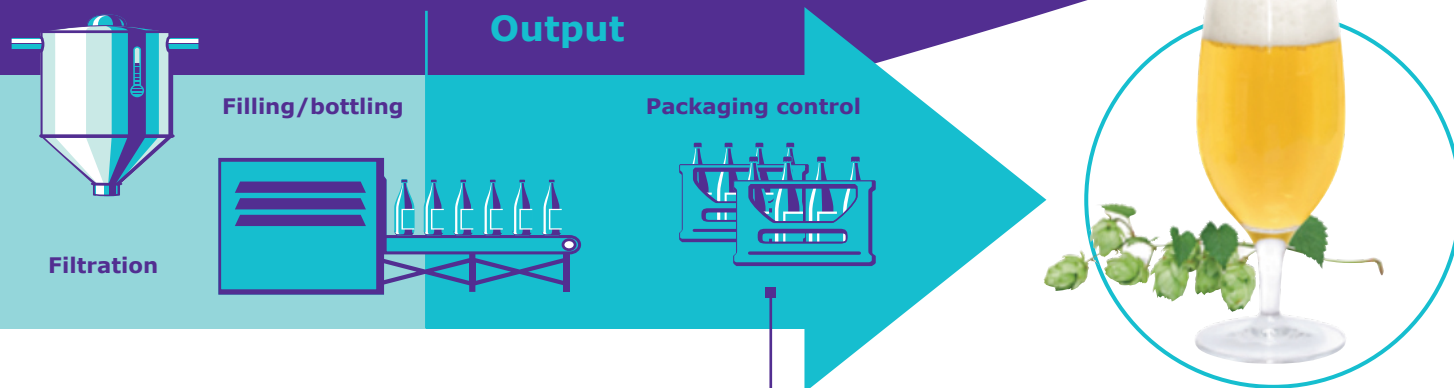

In-Process Control

Semi-quantitative testing

- pH strips and paper
> Page 148
- MQuant™ test strips, e.g. glucose, calcium
> Page 138



Quantitative testing

Test strips

- RQflex® 10
> Page 114
- Reflectoquant® disinfectant parameter test kits, e.g. chlorine
> Page 120



Photometry

- Move 100 and Move Cl₂/O₃/ClO₂/CyA/pH colorimeters
> Page 40
- Spectroquant® test kits, e.g. iron, sulfite
> Page 54



Microbial and pathogen testing

- Air sampler, e.g. MAS-family
> Page 157
- Surface monitoring, e.g. HY-LiTE®, HY-RiSE®
> Page 157



Reference materials

- CRM
> Page 102
- Certipur®
> Page 106




**CHECK
METHODS
FOR BEER
ANALYSIS**

For more information on the preprogrammed methods of beer analysis see page 46



food & beverage workflow

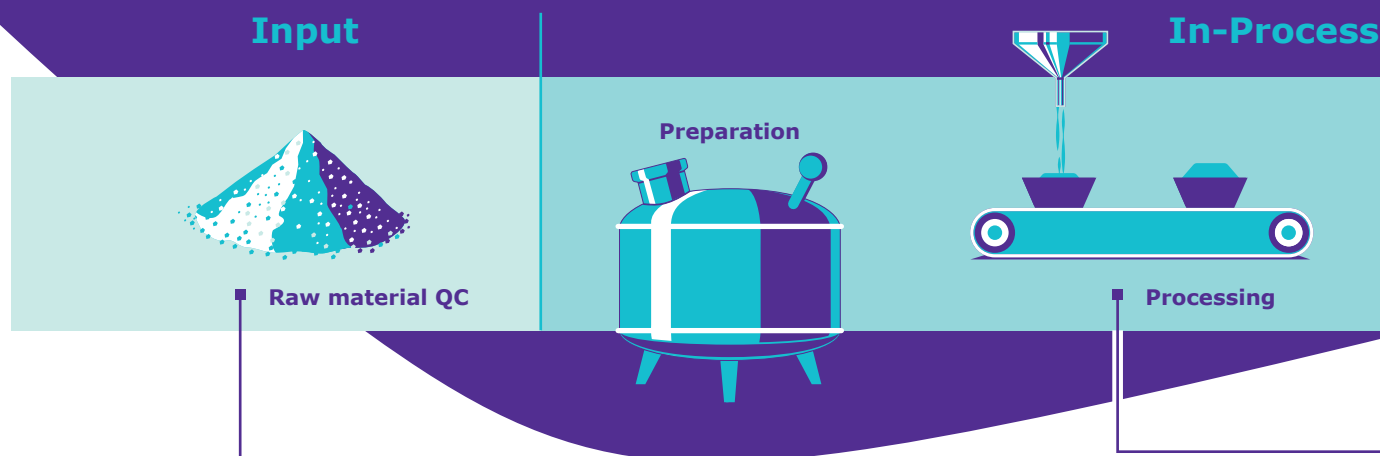

Quality Control

Chromatography

- HPLC, GC, TLC
> Page 158
- Syringe filters
> Page 163



Spectrophotometry

- Spectroquant® Prove 600
> Page 36
- Spectroquant® test kits, e.g. calcium, nitrate, sulfite
> Page 54



Reference materials

- CRM for test kits
> Page 102
- Certipur®
> Page 106
- Standards for pesticides
> Page 160



Microbial and pathogen testing

- Microbial filtration testing, e.g. EZ family
> Page 156
- Culture media, dehydrated and ready-to-use media
> Page 156



Water purification system

- Milli-Q® system
> Page 163




Ingredient and nutritional testing

- Kjeldahl, total dietary fiber
> Page 161
- Flavors and fragrances
> Page 161
- Karl Fischer - reagents
> Page 162

Food and beverage producers face increasing safety regulations, and are required to perform detailed analyses of raw materials, in-process controls, quality tests, and hygiene monitoring. As all of these analyses take time, our rapid and on-the-spot tests for chemical and microbiological contamination are designed to help you get your product to the market faster.

The workflow diagram shows the products you need to accurately analyze important chemical parameters in food and beverages, such as the concentration of ascorbic acid, glucose and fructose, or microbiological contamination.

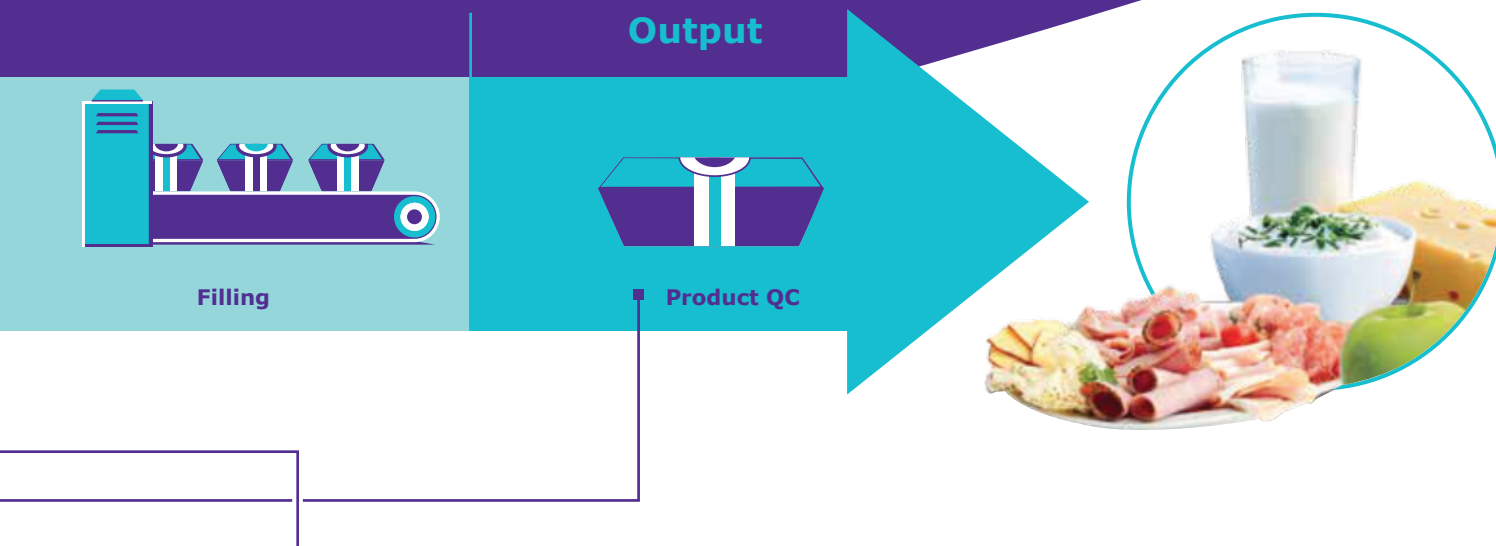

In-Process Control

Semi-quantitative testing

- pH strips and paper
> **Page 148**
- MQuant™ test strips,
e.g. free fatty acids
> **Page 138**



Quantitative testing

Test strips

- RQflex® 10
> **Page 114**
- Reflectoquant® test kits e.g. HMF,
glucose, sucrose, ascorbic acid
> **Page 120**



Photometry

- Move 100 and Move Cl₂/O₃/
ClO₂/CyA/pH colorimeters
> **Page 40**
- Spectroquant® test kits,
e.g. iron, magnesium, sulfite
> **Page 54**



Microbial and pathogen testing

- Air sampler,
e.g. MAS-family
> **Page 157**
- Surface monitoring,
e.g. HY-LiTE®, HY-RiSE®
> **Page 157**




Reference materials

- CRM
> **Page 102**
- Certipur®
> **Page 106**



ANALYTICAL APPLICATION NOTES FINDER



Interested in more application examples? Visit the analytical application notes finder on our website!

www.merckmillipore.com/aaf

JUST PROVE IT!



Is your drinking water safe?

Easy and economical bromate analysis

The application

- Bromate is formed when bromide-rich water is treated with ozone during sterilization
- The analysis of bromate in drinking water is essential because it is a toxic, carcinogenic substance
- Limit according to WHO guidelines: 10 µg/L BrO₃⁻

Our solution: Spectroquant® Prove 600

Spectroquant® Prove 600 offers a super-sensitive photometric method for bromate analysis. When combined with a 100-mm cell, it allows you to easily and accurately detect very low bromate levels, and check if they are within required limits – without high investments.

Benefits

- Easy, accurate and economical solution
- Bromate analysis method acc. to ISO 15061:2001
- Super-sensitive measurement range: 0.5-20 µg/L BrO₃⁻ for evaporated samples, 2.5-100 µg/L BrO₃⁻ without evaporation



Learn more about hassle-free bromate analysis:
www.merckmillipore.com/bromate



Photometry Spectroquant®

General information	34
Instruments	35
Prove spectrophotometers	36
Move colorimeters	40
Multy colorimeter	42
NOVA photometers	43
Accessories	44
Special applications	46
Sample preparation	50
Crack Sets	51
Thermoreactors	52
Test Kits	54
USEPA approved	56
Drinking water guidelines	57
Product list	58
Test Kits for other photometer brands	80
Test Kits for samples with high salt content	82
Quality Assurance	88
CombiCheck	98
Certified Reference Materials	102
Standard solutions	106



Spectroquant® Concept

Complete system for photometric analysis

Test assured

If you want to be certain about your measurements, analytical quality assurance (AQA) is a must. It allows you to prove the validity and reproducibility of your photometric results. With the **Spectroquant® concept**, you can focus on your daily work without worrying about the quality of your results. Our convenient, all-in-one solution includes everything you need for secure analysis, and they work seamlessly together: reliable instruments, high-quality test kits, customized applications, and start-to-finish AQA.

See how our products support your workflow on pages 20-31.

Spectroquant® system

Instruments & accessories Spectroquant® colorimeters and photometers combine high measurement quality with simple handling: Spectroquant® Prove | Spectroquant® Move | Spectroquant® Multy | Spectroquant® NOVA

Sample preparation Simply effective and comfortable with crack sets and thermoreactors: Spectroquant® Crack Set | Spectroquant® Thermoreactors TR 320 / 420 / 620

Test kits More than 200 Spectroquant® test kits offer competent solutions for the widest conceivable range of applications: Reagent test kits | Cell test kits | Test kits for samples with salt content | Test kits for other photometer brands

Quality certificates Quality certificates for each test kit confirm the consistent quality of all batches

Quality assurance Perfect Analytical Quality Assurance (AQA) thanks to certified standards, GLP-compliant documentation, and tools: Spectroquant® PhotoCheck | Certipur® UV/VIS standards | Spectroquant® PipeCheck | Spectroquant® CombiCheck | Standard solutions (CRM) for photometric applications | Certipur® standard solutions

Choose the perfect photometer

*Not sure which photometer is ideal for your daily lab work?
Find out in our photometer selection guide!*

www.merckmillipore.com/photometer-selection-guide



Spectroquant® instruments

Colorimeters

Bar-code reading
No. of test parameters
Mains operation
Battery operation

Spectroquant® Move – Reliable, waterproof colorimeters for rapid, on-site results

Move $\text{Cl}_2/\text{O}_3/\text{ClO}_2/\text{CyA}/\text{pH}$	Perfect colorimeter for disinfection control		5		■
Move 100	Ideal instrument for on-site wastewater and drinking water analysis		>100		■



Spectroquant® Multy – Rechargeable mobile lab colorimeter for routine testing

Multy	Compact and portable for routine measurements of different parameters		>130	■	■
-------	---	--	------	---	---



Photometers

Spectroquant® NOVA – Compact, convenient filter photometers for reliable measurements

NOVA 30 A	Basic instrument for routine measurements in wastewater analysis	■	>60	■	■
NOVA 60	Routine testing of all types of water	■	>180	■	
NOVA 60 A	Same as NOVA 60, but can also be operated with rechargeable powerpack	■	>180	■	■



Spectroquant® Prove – Sophisticated touchscreen photometers for sensitive, secure analysis

Prove 100	Best choice for use with our broad range of Spectroquant® test kits, or for only performing Vis measurements	■	>200		
Prove 300	Equipped with long-lasting xenon lamp for more intensive use, and capable of UV and Vis measurements for greater flexibility in intricate analyses	■	>200		
Prove 600	Designed for high-end UV/Vis optics and cells of up to 100 mm, also offers excellent resolution and sensitivity for use with test kits, complex kinetics or spectral measurements	■	>200		



Spectroquant® Prove Spectrophotometers

Sophisticated analysis made simple

Our goal was to build the perfect tool for water analysis. One that unites the simplicity you want with the security you need, and durability you expect. Spectroquant® Prove delivers all these and more. It offers intuitive controls, and is pre-programmed for over 200 Spectroquant® test kits and methods to make analysis smoother than ever.

Just PRove it.

Long-life lamp with reference beam technology for brilliant durability and economy

Innovative ambient light measurement technology, patent pending

Smart touchscreen for simple navigation in 28 languages

Customize settings set turbidity correction, add dilution factors, or simultaneously display adsorption and concentration

Assign individualized measuring ranges to see if results are within limits

Use the USB or Ethernet ports to connect to your printer or LIMS for fast data transfer

Materials and design are built to last and resistant to most lab chemicals

A small beauty in your lab: 42 cm x 28 cm x 24 cm



Live ID bar codes on cell and reagent tests automatically transfer important data to the spectrophotometer:



- Method recognition
- Lot number
- Expiry date
- Calibration update



Reagent tests include an AutoSelector for automatic test detection and result calculation



Cells in the test kits contain virtually all reagents necessary for the analysis



100 mm 50 mm 20 mm 10 mm

All Prove models detect 10-, 20-, and 50-mm cells



For even greater sensitivity, Prove 600 is also compatible with 100-mm cells



Cell Test Port allows direct insertion of round cells



Removable cell holder for easy cleaning in case of spills



Choose your test

Choose our convenient cell tests or economical reagent tests
> Learn more on page 55

Spectroquant® Prove Spectrophotometers

Three perfect models. Just choose.

100



Spectroquant® Prove 100
Ord. No. 1.73016.0001

For routine applications

Prove 100 is the best choice for those who primarily use our broad range of Spectroquant® test kits, or only perform Vis measurements. High quality and great value for money for your daily analyses.

300



Spectroquant® Prove 300
Ord. No. 1.73017.0001

For sensitive measurements

Thanks to its long-lasting xenon lamp, Prove 300 is ideal for more intensive use. What's more, it is capable of both UV and Vis measurements, so you have greater flexibility for more intricate analyses.

600



Spectroquant® Prove 600
Ord. No. 1.73018.0001

For complex analyses

Designed for high-end UV/Vis optics, and cells of up to 100-mm, Prove 600 packs great power into a compact size. Excellent resolution and sensitivity for use with test kits, complex kinetics or spectral measurements.

Prove 100
Prove 300
Prove 600

Specifications

Measuring technology	Spectrophotometer with reference beam technology	■	■	■
Wavelength range	Vis (320 – 1,100 nm)	■	■	■
	UV (190 – 320 nm)		■	■
Lamp type	Tungsten halogen lamp	■		
	Xenon flash lamp		■	■
Ambient light protection	Measurement with open shaft possible due to proprietary solution (patent pending)	■	■	■
Spectral bandwidth	4 nm	■	■	
	1.8 nm			■
Smart Screen display	Resistive touch screen	■	■	
	P-cap glass touch screen			■
Live ID system	2-D Bar-code recognition for cell tests and reagent tests	■	■	■
	Bar-code contains lot, expiry, and calibration data. Data stored with each measurement	■	■	■
Cell size	16-mm round cells, 10-, 20- and 50-mm rectangular cells with automatic recognition	■	■	■
	100-mm rectangular cells with automatic recognition			■
Cell holder	Removable for easy cleaning	■	■	■
Methods	Programmed methods of all Spectroquant® cell and reagent tests, 99 user defined methods, 20 profiles for kinetics and absorbance scans each	■	■	■
Applications	Free preprogrammed applications: Bromate, Brewery packages (MEBAK/EBC/ASBC methods), Sugar (ICUMSA), Oil (DOBI, olive oil)	■	■	■
AQA Prime	Individual settings for all methods in AQA 1 (instrument check) and AQA 2 mode (system check) and pipette check	■	■	■
Sample matrix check	Easy access through setting menu to perform instrument supported matrix check for each method	■	■	■
Software updates	Free method updates on our website	■	■	■
Languages	Navigation in 28 built-in languages	■	■	■
Communication interfaces	USB: 2 x USB-A (for printer, USB memory devices, keyboard or bar-code reader), 1 x USB-B; Ethernet: LAN connection	■	■	■

Application fields



Wastewater

Regular testing, and the use of cell test kits are common in wastewater analysis. Prove 100 is the perfect choice for these measurements. The Spectroquant® portfolio offers the broadest selection of COD tests. Just choose the measuring range that best suits your needs, and enjoy precise results.

Wastewater workflow

> Page 22



Drinking water & beverages

Analyzing drinking water and beverages usually involves reagent tests as they offer lower detection limits for parameters like manganese and sulfate. Prove 300 is ideal here as it allows UV/Vis analyses, and is programmed with free applications, like bromate and brewery tests.

Drinking water workflow

> Page 24



Process water

Even low levels of impurities in process water can lead to damages, downtime, and costly repairs. To help you avoid these, we offer the most sensitive silicate and chloride tests with the lowest measuring ranges available. For even greater sensitivity, use the 100-mm cell in Prove 600.

Cooling & boiler water workflow

> Page 20

Just ask.

Service and support

We understand the importance of reliable instruments, and the complexities of documentation. That's why we offer a comprehensive service plan that takes care of both.

All Spectroquant® service plans offer the following benefits:

- **Performance check** with reference materials – certificate included
- **Factory-recommended maintenance** to prevent breakdowns
- **Telephone support hotline** connects you to our technical experts
- **Free software upgrades** to keep your instrument up to date
- **Reagent delivery program** for convenient, punctual supply of our high-quality test kits

Contact us today for your personalized Spectroquant® service plan:

www.merckmillipore.com/water-analytics-service



Visit our E-shop

All our products for water, food and environmental analytics are available online – day or night. For further details and easy shopping, please visit www.sigma-aldrich.com

Spectroquant® Move Colorimeters

Rapid, reliable results on-site



Spectroquant® Move 100 Take your lab to the sample

Spectroquant® Move 100 is made for rapid, reliable on-site water analysis. No delays, no risk of sample deterioration and no need for additional instruments. The compact, portable colorimeter covers every important parameter of drinking water and wastewater analysis in one instrument.

- Pre-programmed for over 100 parameters
- Wide choice of measuring ranges for accurate results
- Dust tight and waterproof according to IP 68 classification
- Secure results with simplified AQA and enhanced documentation

get answers
on the move

Spectroquant® Move Cl₂/O₃/ClO₂/CyA/pH Simplify disinfection control

Spectroquant® Move Cl₂/O₃/ClO₂/CyA/pH is built for easy disinfection control in field tests and process monitoring. The small device is automated for five essential parameters of disinfection control – chlorine, ozone, chlorine dioxide, cyanuric acid, and pH – based on Spectroquant® test kits.

- One instrument for all key parameters in disinfection control
- Dust tight and waterproof according to IP 68 classification
- Pre-programmed for high-quality Spectroquant® test kits
- Complete documentation for streamlined AQA and audits



Data Transfer

Easy data transmission (to printer or PC) via the Spectroquant® Data Transfer infrared module.
Order Number: 1.73633.0001



www.merckmillipore.com/photometry

Spectroquant® Move colorimeters

Ord. No.

Spectroquant® Move 100 colorimeter

1.73632.0001

Spectroquant® Move Cl₂/O₃/ClO₂/CyA/pH colorimeter

1.73635.0001

Technical data

Move 100 Move Cl₂/O₃/ClO₂/CyA/pH

Scope of delivery	Instrument in light carrying case, 4 batteries, 3 round vials each 24- and 16-mm ø, 1 adapter for 16-mm vials, screw driver, guarantee certificate, certificate of compliance, instruction manual	■	■
Display	Backlit graphic-display	■	
	Backlit LCD (on keypress)		■
Interfaces	IR interface for data transfer	■	■
	RJ45 connector for internet updates	■	
Optics	LED, interference filter, photosensor, transparent measurement chamber	■	■
Wavelength	430, 530, 560, 580, 610 and 660 nm	■	
	530 nm		■
Wavelength accuracy	±1 nm	■	■
Photometric accuracy	1.000 Abs ±0.020 Abs		
	2.600 Abs ±0.052 Abs (± 2 % FS) (measured with standard solutions – T = 20 – 25°C)	■	
	1.000 ± 0.030 Abs		
	2.600 Abs ± 0.078 Abs (± 3 % FS) 3 % FS (measured with standard solutions – T = 20 – 25°C)		■
Photometric resolution	0.005 A	■	
	0.001 A		■
Operation	Acid and solvent resistant tactile film keyboard	■	■
Power supply	4 batteries (Type AA/LR6), capacity approx. 26 hours continuous use or 3,500 tests	■	
	4 batteries (Type AAA/LR03), capacity approx. 17 hours continuous use or 5,000 tests		■
Weight	approx. 450 g	■	
	approx. 260 g		■
Dimensions	approx. 210 x 95 x 45 mm (instrument)	■	
	approx. 395 x 295 x 106 mm (case)		
	approx. 155 x 75 x 35 mm (instrument)		■
	approx. 340 x 275 x 83 mm (case)		
IP classification	Dust and waterproof acc. to IP 68	■	■
Storage capacity	approx. 1,000 data sets	■	
	Internal ring memory for 16 data sets		■
Comments	CE-Conformity	■	■
Accessories	>> see page 44 Spectroquant® Accessories	■	■

Spectroquant® Multy Colorimeter

Economical routine testing

Spectroquant® Multy

Looking for a comprehensive yet inexpensive colorimeter for photometric water analysis? Spectroquant® Multy is pre-programmed for over 130 Spectroquant® test kits, covering all essential parameters in drinking water and wastewater.

Connection
port

for printing and data transfer

Programmed
methods

for drinking water and wastewater

rechargeable
batteries

for complete mobility



Spectroquant® Multy colorimeter

Ord. No. 1.73630.0001

Scope of delivery	Case, colorimeter, adapter unit for 16-mm round cells, lid for adapter unit, 7 rechargeable batteries, lithium battery (to ensure data storage), interface cable for connection to the PC or printer, 3 x 16 mm round cells, 3 x 24-mm round cells, screw driver (for battery compartment), 100 mL plastic beaker, operating manual
Display	Large format graphic display
Optics	6 temperature compensated LED with interference filters, internal reference channel (dual beam technology)
Measuring wavelength	430 nm, 530 nm, 560 nm, 580 nm, 610 nm, 660 nm
Interface	RS 232 for printer and PC connection
Methods	Programming of more than 130 methods for Spectroquant® cell and reagent tests, as well as physical measurements and pre-programmed applications
Keypad	Acid and solvent resistant, touch-sensitive with audible feedback
Power supply	7 Ni-MH-battery pack (AA/Mignon), charged whilst in the unit with integrated mains charger, integrated overload cut-out.
Ambient conditions	up to max. 90 % humidity (non condensing), approx. 5 – 40°C
System check	automatic selfcheck of the instrument
Storage capacity	for 1,000 data sets, with date, time and registration number
CE approval	yes
Dimensions	approx. 265 x 195 x 70 mm (unit), 440 x 370 x 140 mm (case)
Accessories	>> see page 44 Spectroquant® Accessories

Spectroquant® NOVA Photometers

Convenient, accurate measurements



Spectroquant® NOVA

Enjoy high measurement quality with great simplicity. Spectroquant® NOVA photometers pack maximum convenience into a minimum size.

- Bar-code reading of Spectroquant® tests for auto-recognition of cell size, method and calculation of results
- Compact and mobile for easy transportation between labs
- Variety of measuring ranges and parameters for accurate results
- Instrument-supported AQA

Spectroquant® NOVA photometers	Ord. No.
Spectroquant® NOVA 30 A	1.09748.0001
Spectroquant® NOVA 60	1.09751.0001
Spectroquant® NOVA 60 A	1.09752.0001

Technical data		NOVA 30 A	60	60 A
Wavelength	6 filters in array-technique with reference beam: 340, 445, 525, 550, 605, 690 nm, ± 2 nm half band width 10 nm (30 nm for 340 nm)	■		
	12 filters in array-technique with refer. beam: 340, 410, 445, 500, 525, 550, 565, 605, 620, 665, 690, 820 nm, ± 2 nm half band width 10 nm (30 nm for 340 nm)		■	■
Photometric reproducibility	0.001 A at 1.000 A	■	■	■
Photometric resolution	0.001 A	■	■	■
Types of determination	Absorbance, concentration, transmission	■	■	■
Measuring range of absorbance	-0.300 A to 3.200 A	■	■	■
Lamp	Tungsten halogen lamp, preset, no warm-up time, measuring time 2 s	■	■	■
Date/Time	real time clock integrated in the photometer	■	■	■
Cell compartment	16-mm round cells	■		
	10-, 20- and 50-mm rectangular cells and 16-mm round cells		■	■
Test recognition	AutoSelect function (bar-code reading system) automatic cell recognition	■	■	■
Method-update	via Internet	■	■	■
AQA	3 quality control modes	■	■	■
Turbidity correction	simultaneous multiwavelength measurement to correct turbidity	■	■	■
Interface	RS 232 C serial interface for printer and computer	■	■	■
Methods	Programming of more than 60 methods for Spectroquant® cell tests, as well as physical measurements and pre-programmed applications	■		
	Programming of more than 170 methods for Spectroquant® cell and reagent tests, as well as physical measurements and pre-programmed applications		■	■
Storage capacity	up to 500 results	■		
	up to 1,000 results		■	■
Power supply	100 – 240 V~, 50 – 60 Hz	■	■	■
Temperature	Storage: -25°C to +65°C, operations: +5°C to +40°C	■	■	■
Allowable relative humidity	Annual mean: ≤ 75 %, 30 days/year: 95 %, other days: 85 %	■	■	■
Dimensions	140 x 270 x 260 mm (H x D x W)	■	■	■
Weight	2.8 kg incl. battery	■		■
	2.3 kg	■	■	
Special functions	50 free programmable methods		■	■
Accessories	>> see page 44 Spectroquant® Accessories	■	■	■

Spectroquant® Accessories

Economical routine testing



Cells for Spectroquant® instruments

Product	Prove 100	Prove 300	Prove 600	NOVA	Multy	Move	Ord. No.
Empty 16-mm round cells with screw cap	■	■	■	■	■	■	1.14724.0001
Empty 24-mm round cells with screw caps					■	■	1.73650.0001
Rectangular cells 10-mm	■	■	■	■			1.14946.0001
Rectangular cells 20-mm	■	■	■	■			1.14947.0001
Rectangular cells 50-mm	■	■	■	■			1.14944.0001
Rectangular cells 100-mm			■				1.74011.0001
Rectangular cells quartz 10-mm	■	■	■	■			1.00784.0001
Semi-microcells 50 mm	■	■	■	■			1.73502.0001

Accessories for Spectroquant® instruments

Product	Ord. No. for Prove	Ord. No. for NOVA	Ord. No. for Move
Case	1.73020.0001	1.09769.0001	included
Halogen lamp module	1.74010.0001 (for Prove 100)	1.09749.0001	
Power supply	1.74064.0001	1.09734.0001 1.09779.0001 (EU adapter) 1.20097.0001 (US adapter) 1.20347.0001 (UK adapter) 1.20497.0001 (AUS adapter)	4 batteries included
Positioning aid		1.00787.0001 (for 10 mm cells)	
Data transfer	No accessories needed	1.14964.0001 (PC software)	1.73633.0001 (unit, cable and software)
PC cable		1.14667.0001 (for serial bus)	1.73634.0001 (for updates)



plug and prove

Only for Spectroquant® Prove: Commercially available
USB hubs, USB handheld bar-code scanners and PC
keyboards can be connected via the USB port

keep it clean!



Reliable and residue-free cleaning with Extran®

Clean instruments and labware are essential for accurate measurements. Extran® is a reliable and residue-free cleaning agent of consistent composition, so you won't have to frequently modify your process and applications.

Easy cleaning

- Thoroughly wash labware with water, then rinse with distilled water
- Use a dry cloth to wipe off any stains or marks on surfaces
- Remove grease marks by immersing the vessel in 2-5% Extran®, then rinse with distilled water

Cleaning agents for cells and glass vessels

Extran® detergent MA 02

Ord. No. 1.07553.2500

Neutral, contains phosphates

pH of 2-5 % solutions approx. 7.2-7.5

Extran® detergent MA 05

Ord. No. 1.40000.2500

Alkaline, phosphate-free | Not for alkali-sensitive material such as aluminium
pH of a 2-5 % solution approx. 11.6-12.0

Cleaning validation

The Spectroquant® surfactants (non-ionic) cell test (page 76) supports effective cleaning validation.

Clean enough for chlorine testing?

Why is it so important to rinse cells with sulfuric acid 25% for chlorine testing?

Reagent 2 of the total chlorine test contains potassium iodide, which has a very high affinity to glass surfaces, and will remain on the glass if only cleaned with distilled water. Due to the residual potassium iodide, results for free chlorine will be too high, and those for total chlorine will be too low.

Our solution: Sulfuric acid 25%

Cleaning glassware when measuring total chlorine (Ord. No. 1.00597.0001 / 1.00599.0001): After each total chlorine determination, rinse the cell with sulfuric acid 25%, then several times with distilled water.

Spectroquant® Prove Special applications

Brewery methods

	Determination	Measuring range	Method	Prove		
				100	300	600
A	∂ Acids	0–80 mg/L	Own coloring	■	■	■
	Anthocyanogens (Harris and Ricketts method)	0–100 mg/L	Acidic hydrolysis	■	■	■
B	Bitterness – Beer (EBC method)	1–80 BU	UV-absorption		■	■
	Bitterness – Wort (EBC method)	1–120 BU	UV-absorption		■	■
C	Color (EBC method)	0.0–60.0 EBC Units	Own coloring	■	■	■
	Copper (EBC method)	0.10–5.00 mg/L Cu	Cuprethol	■	■	■
F	Flavanoids (EBC method)	3.0–200.0 mg/L	4-(Dimethylamino)-cinnamaldehyde	■	■	■
	Free Amino Nitrogen (Beer/Wort)	0–400 mg/L	Ninhydrin	■	■	■
I	Iso-∂ Acids	0–60 mg/L	UV -absorption		■	■
	Iron (EBC method)	0.000–1.000 mg/L Fe	Ferrospectral®	■	■	■
	Iron (EBC method)	0.000–0.800 mg/L Fe	Ferrospectral®	■	■	■
N	Nickel (EBC method)	0.00–5.00 mg/L Ni	Dimethylglyoxime	■	■	■
P	Photometric Iodine Test	0.00–0.80	Iodine	■	■	■
R	Reducing Power, spectrophotometric	0–100%	DPI	■	■	■
S	Steam-volatile Phenols Malt	0.00–3.00 mg/kg	Aminoantipyrine extractive	■	■	■
	Beer	0.00–0.30 mg/kg				
T	Thiobarbituric Acid Number (TAN)	0–250 TAN	Thiobarbituric acids	■	■	■
	Total Carbohydrates (EBC method)	0.000–6.000 g/100 mL	Anthrone	■	■	■
	Total Polyphenols (EBC method)	0–800 mg/L	Iron (III)	■	■	■
V	Vicinal Diketones	0.00–1.00 mg/kg	Phenylenediamine	■	■	■



The new Spectroquant® Prove software package, "Analysis methods for the brewery industry", contains all 21 methods required for complete beer analysis – from raw materials to finished product. The test procedures follow MEBAK (Mittleeuropäische Brautechnische Analysenkommission), EBC (European Brewery Convention) or ASBC (American Society of Brewing Chemists) methods.

To further support your analysis, the accompanying manual provides step-by-step instructions for reagent preparation, sample processing and analysis. The package also includes information about test solution stability and storage, which aren't provided in the standard MEBAK method description.

ANALYTICAL APPLICATION NOTES FINDER

Besides test kits, we also provide detailed application notes to support your analysis. Learn more on:
www.merckmillipore.com/aaf > Photometry



Visit our E-shop

All our products for water, food and environmental analytics are available online – day or night. For further details and easy shopping, please visit www.sigma-aldrich.com

www.merckmillipore.com/photometry

Chemical and physical applications

	Determination	Measuring range	Method	Prove		
				100	300	600
A	Ammonia, free	0.00–3.65 mg/L NH ₃	Indophenol blue	■	■	■
B	Bromate in water / drinking water	0.5–200 µg/L BrO ₃	3,3'-dimethylnaphtidine	■	■	■
C	Chlorophyll-a (DIN/ISO)	0–50,000 µg/L Chl-a, Phaeo	Analogous DIN 38412, ISO 10260	■	■	■
	Chlorophyll-a (APHA/ASTM)	0–50,000 mg/m ³ Chl-a, Phaeo	Analogous APHA 10200-H, ASTM D3731-87	■	■	■
	Chlorophyll-a, -b, -c	0–50,000 mg/m ³ Chl-a, Chl-b, Chl-c	Trichromatic method, analogous APHA 10200-H, ASTM D3731-87	■	■	■
	Cobalt in Water	0.5–10.0 mg/L Co	Nitroso-R-Salt	■	■	■
M	Mercury in water / wastewater	0.025–1.000 mg/L Hg	Michler's thioketone	■	■	■
N	Nitrate (UV)	0.0–7.0 mg/L NO ₃ -N	Analogous to APHA 4500-NO ₃ -B		■	■
P	Palladium in water / wastewater	0.05–1.25 mg/L Pd	Michler's thioketone	■	■	■
	Platinum in water / wastewater	0.10–1.25 mg/L Pt	1,2-phenyldiamine	■	■	■
S	Spectral Absorption Coefficient $\alpha(254)$	0.5–250 m ⁻¹	Physical measurement according DIN 38404, at 254 nm		■	■
	Spectral Absorption Coefficient $\alpha(436)$	0.5–250 m ⁻¹	Physical measurement according DIN 7887, at 436 nm	■	■	■
	Spectral Attenuation Coefficient $\mu(254)$	0.5–250 m ⁻¹	Physical measurement according DIN 38404, at 254 nm		■	■
	Suspended Solids	25–750 mg/L susp. solids	Physical measurement	■	■	■

ICUMSA and oil determination

Spectroquant® Prove photometers offer special applications for testing the quality of palm oil, olive oil, or sugar, based on methods recommended by the relevant regulatory agencies. In addition to over 180 pre-programmed methods, we provide supplementary application software for more specific requirements in quality control. The packages ensure that you have accurate results in compliance with international standards.

	Determination	Measuring range	Method	Prove		
				100	300	600
C	Carotene Palm Oil	10–7,500 mg/kg β -Car	Own coloring	■	■	■
D	DOBI Palm Oil	0.00–4.00 DOBI	UV-absorption		■	■
K	K232 Olive Oil	0.00–4.00 K ₂₃₂	UV-absorption		■	■
	K268 Olive Oil	0.00–4.00 K ₂₆₈	UV-absorption		■	■
	K270 Olive Oil	0.00–4.00 K ₂₇₀	UV-absorption		■	■
	delta K268 Olive Oil	-0.10–1.00 ΔK_{268}	UV-absorption		■	■
	delta K270 Olive Oil	-0.10–1.00 ΔK_{270}	UV-absorption		■	■
I	ICUMSA Color GS1/3-7	0–50,000 IU _{7.0}	Own coloring	■	■	■
	ICUMSA Color GS2/3-9	0–600 IU _{7.0}	Own coloring	■	■	■
	ICUMSA Color GS2/3-10	0–50 IU _{7.0}	Own coloring	■	■	■
	ICUMSA Color GS9/1/2/3-8	0–20,000 IU _{7.0}	Own coloring	■	■	■

Spectroquant® Prove Special applications

New color determinations

Spectroquant® Prove spectrophotometers support color determination in a variety of samples, such as beer, lubricants, oils or food products.

Determination		Description*	Prove 100 300 600
A	ASTM Color	Determination of the color of a wide variety of petroleum products (lubricating oils, heating oils, diesel fuel oils, petroleum waxes)	Q1 2017
C	Color (ASBC)	Determination of the color of brewery products according to ASBC (American Society of Brewing Chemists)	Q3 2017
	Color (436)	Measurement at 436 nm, range 0.1-250 m ⁻¹	■ ■ ■
	Color (525)	Measurement at 525 nm, range 0.1-250 m ⁻¹	■ ■ ■
	Color (620)	Measurement at 620 nm, range 0.1-250 m ⁻¹	■ ■ ■
	Color (410) (EN 7887)	Measurement at 410 nm, range 2-2,500 mg/L Pt	■ ■ ■
	Color, Hazen	Physical measurement, corresponds to APHA 2120 B, DIN EN ISO 6271-2, at 340 nm, range 0.2 – 500 mg/L Pt, Pt/Co, Hazen, CU	■ ■ ■
	Color, Hazen	Physical measurement, corresponds to APHA 2120 B, DIN EN ISO 6271-2, at 445 nm, range 0 – 1,000 mg/L Pt, Pt/Co, Hazen, CU	■ ■ ■
	Color, Hazen	Physical measurement, corresponds to APHA 2120 B, DIN EN ISO 6271-2, at 455 nm, range 0 – 1,000 mg/L Pt, Pt/Co, Hazen, CU	■ ■ ■
	Color, Hazen	Physical measurement, corresponds to APHA 2120 B, DIN EN ISO 6271-2, at 3465 nm, range 0 – 1,000 mg/L Pt, Pt/Co, Hazen, CU	■ ■ ■
	C*ab colorfulness CIE 1976	Evaluation of color coordinates according to the CIELAB color space	Q3 2017
	Color difference delta E*ab (CIE)	Evaluation of color differences according to the CIELAB color space	Q3 2017
	Color difference delta L* (CIE)		Q3 2017
	Color difference delta a* (CIE)		Q3 2017
	Color difference delta b* (CIE)		Q3 2017
	Color difference delta C*ab (CIE)		Q3 2017
	Color difference delta E*ab (Hunter)	Evaluation of color differences according to the HunterLab color space	Q3 2017
	Color difference delta L* (Hunter)		Q3 2017
	Color difference delta a* (Hunter)		Q3 2017
	Color difference delta b* (Hunter)		Q3 2017
	Color difference delta C*ab (Hunter)		Q3 2017
G	Gardner Color	Estimation of color by the Gardner color scale – clear, yellow-brown liquids, e.g. drying oils, varnishes, solutions of fatty acids, resins etc.	Q1 2017
H	Hess-Ives color units	Spectrophotometric determination of the Hess-Ives color units	Q3 2017
I	Iodine Color Number, lower range	Measurement at 340 nm, corresponds to DIN 6162 A, range 0.010 – 3.00	■ ■ ■
	Iodine Color Number, higher range	Measurement at 445 nm, corresponds to DIN 6162 A, range 0.2 – 50.0	■ ■ ■
K	Klett color	Spectrophotometric determination of Klett color comparable with the Klett-Summerson colorimeter	Q3 2017
L	L*a*b CIE 1976	Evaluation of color coordinates according to CIELAB 1976	Q3 2017
	L*u*v CIE 1976		Q3 2017
	L * lightness CIE 1976		Q3 2017
	L*a*b Hunter	Evaluation of color coordinates according to the HunterLab color space	Q3 2017

	Determination	Description*	Prove		
			100	300	600
S	Spectral Attenuation coefficient with turbidity correction	Determination of the spectral attenuation coefficient in the range of UV radiation of an unfiltered sample including turbidity correction	Q3 2017		
	Saybolt Color	Determination of the color of refined oils (undyed motor & aviation gasoline, jet propulsion fuels, naphthas, kerosene & petroleum waxes & pharmaceutical white oils)	Q1 2017		
T	Tint index	Determination of Tint index from instrumentally measured Color Coordinates according to ASTM E 313-15e1	Q3 2017		
	Transmittance	Spectrophotometric characterization of optically clear colored liquids	Q3 2017		
U	UV absorbing organic constituents	Spectrophotometric determination of UV absorbing organic constituents at 254 nm	Q3 2017		
	UV absorption	Spectrophotometric determination at 254 nm	Q3 2017		
	UV transmittance	Spectrophotometric determination at 254 nm	Q3 2017		
W	Whiteness index	Determination of Whiteness index from instrumentally measured Color Coordinates according to ASTM E 313-15e1	Q3 2017		
X	xyY color space (CIE color space)	Evaluation of color coordinates according to the CIELAB color space	Q3 2017		
Y	Yellowness index	Determination of Yellowness index from instrumentally measured Color Coordinates according to ASTM E 313-15e1	Q3 2017		

* Measuring ranges will be determined during application development

Stay up to date

New anionic surfactants cell test – superior sensitivity, easier handling

Surfactants enter water systems due to extensive use in detergents and industrial processes. As they can be harmful for humans, animals and vegetation, authorities require regular wastewater testing and treatment to confirm that surfactant content is within limits. The three main classes of surfactants are anionic, cationic and nonionic. The anionic are the most challenging as they are only partly digested by bacteria during water treatment. For greater accuracy, the new Spectroquant® cell test for anionic surfactants offers higher sensitivity and easier handling.

Update to the latest versions:

- Surfactants (anionic) Cell Test [Ord. No 1.02552.0001]
- Surfactants (cationic) Cell Test [Ord. No 1.01764.0001]
- Surfactants (nonionic) Cell Test [Ord. No 1.01787.0001]



Spectroquant® Sample Preparation

Perfectly prepared

Our test kits already contain all the reagents you need for sample preparation and analysis, when decomposition is required. However, for some parameters digestion is not always required. Then you can choose our economical, reliable **Spectroquant® Crack Sets**. They contain only the digestion chemicals you need with clear, easy instructions. For optimal sample preparation, we also offer a range of **Spectroquant® thermoreactors**. They combine outstanding precision and speed to ensure thorough digestion.

Quick
and easy

sample preparation
for analysis

step
by step

instructions with
no special training

All the reagents
you need for digestion



Spectroquant® Crack Sets

Total content determination

Spectroquant® Crack Sets

We offer a choice of three Crack Sets for determining the total content of different parameters. Each set contains all reagents needed for digestion.



Crack Set 10 Crack Set 10C Crack Set 20

Spectroquant®	Crack Set 10 Ord. No. 1.14687.0001	Crack Set 10 C Ord. No. 1.14688.0001	Crack Set 20 Ord. No. 1.14963.0001
Digestions	100	25	90
Sample preparation for determination of total content of	Cd, Cr, Co, Fe, Pb, Ni, P, Zn	Cd, Cr, Co, Fe, Pb, Ni, P, Zn	Nitrogen
Contents	Digestion reagent Acid Neutralizing agent for pH adjustment	Digestion reagent prefilled 16 mm ø cells Acid Neutralizing agent for pH adjustment	Digestion reagent Lye
Accessories	Empty cells 16 mm ø with screw caps Ord. No. 1.14724.0001		Empty cells 16 mm ø with screw caps Ord. No. 1.14724.0001

b e s u r e

Accurate analysis of all wastewater parameters with Spectroquant® test kits

Each country or region has different regulations and limits regarding wastewater parameters. Where can you get the test parameter you want with the exact limits you need? Merck offers the perfect solution: convenient cell tests and economical reagent tests for all wastewater parameters. Combine our high-quality test kits with Spectroquant® Prove spectrophotometers for fast, easy and accurate analysis.

Parameters: Ammonium, COD, Nitrate, Nitrite, Nitrogen (total), Phosphorus (total), Lead, Cadmium, Chromium, Copper, Nickel, Chloride, Sulfate

Learn more on pages 58-79

Spectroquant® Thermoreactors

Consistent, thorough digestion

Developed in practice for practice, **Spectroquant® thermoreactors** offer everything you need for perfect sample preparation: reliability, simplicity, safety and future compatibility. Choose from pre-installed programs to avoid errors in routine use, or program your own methods for complete flexibility.



Flexible selection

between standard and individual programs

easy handling

with our clear digestion guide

two
temperature zones
in one
instrument (TR 620)

Spectroquant® thermoreactors offer 8 pre-installed digestion programs for routine use

Temperature	Time	Method
148°C	120 min	for COD
148°C	20 min	for COD (rapid digestion method)
150°C	120 min	for COD acc. to USEPA
120°C	120 min	for TOC
120°C	60 min	for total nitrogen, total contents of Cr, Cu, Ni, Pb, Cd, Fe, Zn and Ag
120°C	30 min	for AOX and total phosphorus, cyanide
100°C	60 min	
100°C	30 min	

A description of digestion procedures is provided in the instruction sheets included with the test kits. Special digestion variants can be downloaded from: www.merckmillipore.com/aaf

320

**Spectroquant® TR 320****Ord. No. 1.71200.0001****Standard model for basic use**

12 holes | 8 pre-installed programmes

420

**Spectroquant® TR 420****Ord. No. 1.71201.0001****Advanced device for frequent use**

24 holes | 8 pre-installed and 8 freely selectable programmes

620

**Spectroquant® TR 620****Ord. No. 1.71202.0001****Two-in-one instrument for flexible use**

2 x 12 holes | 8 pre-installed and 8 freely selectable programmes | 2 heating zones, which can be controlled separately

Technical data		Spectroquant® thermoreactors		
		TR 320	TR 420	TR 620
Scope of delivery	Incl. integrated protective hood for the determination of COD and TOC, as well as of total contents of cadmium, chromium, copper, cyanide, iron, lead, nickel, nitrogen, phosphorus, silver, and zinc.	■	■	■
Display	LCD display for temperature and time, desired and actual values for heating time and temperature continually shown in the LCD display	■	■	■
Heater	On/off display (the LED blinks red during the heating phase and is permanently on during the digestion phase), contact guard on the surface of the heating-block	■	■	■
Functions	8 pre-installed programs	■	■	■
	8 freely selectable programs		■	■
	Simultaneous digestion of 12 samples	■		
	Simultaneous digestion of 24 samples		■	■
	Free temperature and time selection		■	■
	Two separate temperature-selectable heating zones			■
	Thermosensor and PC cable available		■	■
Holes	AQA documentation for control purposes		■	■
	12 for cell tests ø 16 mm	■		
	24 for cell tests ø 16 mm		■	
Temperature selection	24 (2 x 12) for cell tests ø 16 mm			■
	100°C, 120°C, 148°C and 150°C ±1.0°C	■	■	■
Controlling accuracy	Room temperature–170°C ±1.0°C		■	■
	±1°C ±1 digit	■	■	■
Timer	0 – 180 min freely selectable		■	■
Heating time	8 temperature heating-time programs for simplest possible operation: 148°C (20 min or 120 min), 150°C (120 min), 120°C (30 min, 60 min or 120 min), 100°C (30 + 60 min) automatic power switch-off at the end of the heating time	■	■	■
Mains version	115 V~ / 230 V~, 50 Hz / 60 Hz convertible	■	■	■
Dimensions	180 x 245 x 292 mm (H x W x D)	■	■	■
Weight	2.85 kg	■		
	3.6 kg		■	■
Optional accessories	Thermosensor: heating-block temperature-monitoring option via integrated serial interface and control software for AQA, brass adapter with integrated Pt sensor fitting the holes incl. connector cable (for checking equipment)		■	■

Thermosensor for thermoreactors TR 420/620**Ord. No. 1.71203.0001**

The thermosensor measures the current temperature in the bore of the thermoreactor and compares it with the specified temperature. The results can be transmitted to a PC for documentation purposes.

PC cable for thermoreactors TR 420/620**Ord. No. 1.71204.0001**

Spectroquant® Test Kits

For swift, secure analysis, there's no better choice than Spectroquant® test kits. Consisting of validated, standard-compliant reagents, the kits are pre-programmed for use with Spectroquant® instruments to ensure rapid, reliable results. Thanks to their excellent quality, most of our kits conform to international standards, allowing you to test with absolute confidence.

Be sensitive

Do you need to detect parameters in ultra low concentrations?
With Spectroquant® Prove 600 and 100-mm cells, you can accurately measure the lowest analyte concentrations possible photometrically.



Super-sensitive test kits

Iron Test [Ord. No. 1.14761.0001]

0.0005–5.00 mg/L Fe | 10-, 20-, 50- and 100-mm cells

Phosphate Test [Ord. No. 1.14848.0001]

0.0005–5.00 mg/L PO₄-P | 10-, 20-, 50- and 100-mm cells

Silicate (Silicic Acid) Test [Ord. No. 1.01813.0001]

0.00025 – 0.5000 mg/L SiO₂ | 50- and 100-mm cells

Secure analysis

with validated,
standard-compliant reagents

Bar-code identification

for fast, simple operation

Rapid, reliable results

though pre-programmed blank values

Reagent test kits

- Contain highly stable, ready-to-use reagent mixtures
- AutoSelector uses bar-code system to automatically select the right analysis method in Spectroquant® NOVA and Prove photometers
- Measuring range can be easily varied by selecting the appropriate cell format
- Package insert explains reaction principle, working procedures and application areas
- Long shelf life of up to three years at room temperature



Cell test kits

- Contain virtually all reagents necessary for the analysis
- Spectroquant® NOVA and Prove photometers automatically recognize the test and select the correct analysis method
- Test kit label provides all important information regarding contents, safety and batch number
- Package insert explains reaction principle, working procedures and application areas
- Long shelf life of up to three years at room temperature



Spectroquant® Test Kits

Regulations and approved methods

Testing water according to national regulations or USEPA methods

Since contaminated water is harmful for humans and the environment, regulatory agencies, like the USEPA (U.S. Environmental Protection Agency), require the use of official methods when testing drinking water and wastewater. To support your analysis, many Spectroquant® test kits are developed according to approved USEPA or ISO standards. This ensures that you have reliable, reproducible results that are in compliance with regulations.

USEPA

USEPA-approved: Methods are identical to those from USEPA methods; a copy of the USEPA acceptance letter is available upon request.

USEPA-equivalent: The test kit is validated according to defined procedures; the chemistry is equivalent to USEPA or APHA methods.

**USEPA
approved**

Our "USEPA approved" stamp will help you easily find the right Spectroquant® test kits in the following tables.

The tables also provide references to norms and standards on approved and equivalent methods.



For further information please visit:
www.merckmillipore.com/usepa



We are the first
European company

*to offer a broad range of approved photometric test kits for
drinking water, wastewater and environmental analysis.*

Do you monitor the quality of drinking water?

The following table provides a comparison of a selection of parameters for concentrations listed by the WHO, European Union and USEPA.

Parameter		WHO Guideline	EU	USEPA
From		2011	Oct. 2015	May 2009
A	Aluminium (Al)	not provided	0.2 mg/L	0.05–0.2 mg/L
	Ammonium (NH ₄)	not provided	0.5 mg/L	
	Antimony	0.02 mg/L	0.005 mg/L	0.006 mg/L
	Arsenic (As)	0.01 mg/L	0.01 mg/L	0.01 mg/L
B	Barium (Ba)	0.7 mg/L		2 mg/L
	Boron (B)	2.4 mg/L	1 mg/L	
	Bromate	0.01 mg/L	0.01 mg/L	0.01 mg/L
C	Cadmium (Cd)	0.003 mg/L	0.005 mg/L	0.005 mg/L
	Chloride (Cl ⁻)	not provided	250 mg/L	250 mg/L
	Chlorine (Cl ₂) free	0.2 mg/L (minimal residual concentration at the point of delivery)		4 mg/L
	Chlorine (total)	0.2–1 mg/L		
	Chlorine dioxide (ClO ₂)	not provided		0.8 mg/L
	Chromium (Cr)	0.05 mg/L	0.05 mg/L	0.1 mg/L
	Coliforms (total) (organisms/100 mL)	0	0	5 %
	Color	acceptable	acceptable	15 color units
	Conductivity		2500 µS/cm	
	Copper (Cu)	2 mg/L	2 mg/L	1 mg/L
	Cyanides (Cy)	not provided	0.05 mg/L	0.2 mg/L
F	Fluoride (F ⁻)	1.5 mg/L	1.5 mg/L	4 mg/L
I	Iron (Fe)	not provided	0.2 mg/L	0.3 mg/L
L	Lead (Pb)	0.01 mg/L	0.01 mg/L	0.015 mg/L
M	Manganese (Mn)	not provided	0.05 mg/L	0.05 mg/L
	Mercury (Hg)	0.006 mg/L	0.001 mg/L	0.002 mg/L
	Monochloramines (as Cl ₂)	3 mg/L		
	Molybdenum (Mo)	not provided		
N	Nickel (Ni)	0.07 mg/L	0.02 mg/L	
	Nitrates	50 mg/L (as NO ₃ ⁻)	50 mg/L (as NO ₃ ⁻)	10 mg/L (as N)
	Nitrites	3 mg/L (as NO ₂ ⁻)	0.5 mg/L (as NO ₂ ⁻)	1 mg/L (as N)
P	pH	not provided	6.5–9.5	6.5–8.5
S	Selenium (Se)	0.04 mg/L	0.01 mg/L	0.05 mg/L
	Silver (Ag)	not provided		0.1 mg/L
	Sodium (Na)	not provided	200 mg/L	
	Sulfate (SO ₄)	not provided	250 mg/L	250 mg/L
T	Total Dissolved Solids (TDS)	not provided		500 mg/L
	Trihalomethans (total)	Chloroform: 0.3 mg/L Bromoform: 0.1 mg/L Dibromochloromethane (DBCM): 0.1 mg/L Bromodichloromethane (BDCM): 0.06 mg/L	0.1 mg/L	0.08 mg/L

WHO Guidelines for Drinking Water Quality, 4th edition (**not provided** means that the WHO has not provided guidelines for the parameter, as it is not found at levels posing a health concern in drinking water)

EU Drinking Water Directive of the European Union (Council Directive 98/83/EC), consolidated with the latest amendments of October 2015

USEPA National Primary Drinking Water Regulations and Secondary Drinking Water Standards, May 2009

Spectroquant® Test Kits

Parameters A

	Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
		Prove 100/300/600	NOVA 30/60	Multy	Move 100			
A	Absorbance	-3.300 – 3.300 A	-0.300 – 3.000 A	-2.600 – 2.600 A	-2.600 – 2.600 A	–	–	
	Acid Capacity Cell Test to pH 4.3 (total alkalinity) ^{A)}	0.40 – 8.00 mmol/L	0.40 – 8.00 mmol/L	0.40 – 8.00 mmol/L	0.40 – 8.00 mmol/L	CaCO ₃	120	1.01758.0001
	ADMI Color measurement							
	Alkalinity (total)							
	Aluminium Cell Test	0.02 – 0.50	0.02 – 0.50	0.05 – 0.50	0.05 – 0.50	Al	25	1.00594.0001
	Aluminium Test	0.020 – 1.20	0.020 – 1.20	20 – 700 µg/L	20 – 700 µg/L	Al	350	1.14825.0001
	Ammonia, free	0.000 – 3.00 0.000 – 3.65	–	–	–	NH ₃ -N NH ₃	–	–
USEPA approved	Ammonium Cell Test ^{B.3)}	0.010 – 2.000 0.01 – 2.58 0.010 – 2.000 0.01 – 2.43	0.010 – 2.000 0.01 – 2.58	10 – 2,000 µg/L 10 – 2,576 µg/L	10 – 2,000 µg/L 10 – 2,576 µg/L	NH ₄ -N NH ₄ NH ₃ -N NH ₃	25	1.14739.0001
USEPA approved	Ammonium Test ^{B.3)}	0.010 – 3.00 0.013 – 3.86 0.010 – 3.00 0.016 – 3.65	0.010 – 3.00 • 0.013 – 3.86 •	0.02 – 1.30 0.03 – 1.67	0.02 – 1.30 0.03 – 1.67	NH ₄ -N NH ₄ NH ₃ -N NH ₃	250 500	1.14752.0002 1.14752.0001
USEPA approved	Ammonium Cell Test ^{B.3)}	0.20 – 8.00 0.26 – 10.30 0.20 – 8.00 0.24 – 9.73	0.20 – 8.00 0.26 – 10.30	0.20 – 8.00 0.26 – 10.30	0.20 – 8.00 0.26 – 10.30	NH ₄ -N NH ₄ NH ₃ -N NH ₃	25	1.14558.0001
USEPA approved	Ammonium Cell Test ^{B.3)}	0.5 – 16.0 0.6 – 20.6 0.5 – 16.0 0.6 – 19.5	0.5 – 16.0 0.6 – 20.6	–	–	NH ₄ -N NH ₄ NH ₃ -N NH ₃	25	1.14544.0001
USEPA approved	Ammonium Test ^{B.3)}	2.0 – 150 2.6 – 193 2.0 – 150 2.4 – 182	2.0 – 150 • 2.6 – 193 •	1.0 – 50.0 1.3 – 64.4	1.0 – 50.0 1.3 – 64.4	NH ₄ -N NH ₄ NH ₃ -N NH ₃	100	1.00683.0001
USEPA approved	Ammonium Cell Test ^{B.3)}	4.0 – 80.0 5.2 – 103.0 4.0 – 80.0 4.9 – 97.3	4.0 – 80.0 5.2 – 103.0	4.0 – 80.0 5.2 – 103.0	4.0 – 80.0 5.2 – 103.0	NH ₄ -N NH ₄ NH ₃ -N NH ₃	25	1.14559.0001
	Antimony	0.10 – 8.00	0.10 – 8.00	–	–	Sb	–	–
	AOX Cell Test	0.05 – 2.50	0.05 – 2.50	0.05 – 2.50	0.05 – 2.50	AOX	25	1.00675.0001
	AOX Sample Preparation Set	–	–	–	–	–	25	1.00677.0001
	AOX Enrichment Set	–	–	–	–	–	2	1.00678.0001

A. The cell test contains four 16 mm cells with a bar-code label. After measurement, the cells can be emptied and cleaned for subsequent measurements. | B. This method is officially recognized by the USEPA as an alternative method for the investigation of 1. wastewater, 2. drinking water 3. drinking water and wastewater. | • Only with NOVA 60



Visit our E-shop

All our products for water, food and environmental analytics are available online – day or night. For further details and easy shopping, please visit: www.sigma-aldrich.com

www.merckmillipore.com/photometry

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
own coloring	physical measurement	-	10, 20, 50	-	
Indicator	-	4.0 + 1.0 + 0.5	-	±0.29 mmol/L	2, 5, 9, 10, 11, 13, 15, 18
	see Color, ADMI				
	see Acid Capacity Cell Tests to pH 4.3				
Chromazurol S	analogous APHA 3500-Al B, DIN ISO 10566	0.25 + 6.0	-	±0.02	1, 6, 8, 9, 11, 13, 15, 16, 17, 18
Chromazurol S	analogous APHA 3500-Al B, DIN ISO 10566	0.25 + 1.2 + 5.0	10, 20, 50	±0.009	1, 6, 9, 11, 13, 15, 16, 17, 18
-	Application, measurement of free ammonia under consideration of the pH and temperature of the sample after spectrophotometric determination of the ammonium content, additionally required 1.14752	0.6 + 5.0	10, 20, 50	-	2, 9, 13, 18
Indophenol blue	analogous EPA 350.1, APHA 4500-NH ₃ F, ISO 7150-1, DIN 38406-5	5.0	-	±0.050	1, 2, 5, 9, 11, 12, 13, 15, 17, 18
Indophenol blue	analogous EPA 350.1, APHA 4500-NH ₃ F, ISO 7150-1, DIN 38406-5	0.6 + 5.0	10, 20, 50	±0.016	1, 2, 5, 9, 11, 12, 13, 15, 16, 17, 18
Indophenol blue	analogous EPA 350.1, APHA 4500-NH ₃ F, ISO 7150-1, DIN 38406-5	1.0	-	±0.19	1, 2, 5, 6, 8, 9, 11, 12, 13, 15, 16, 18
Indophenol blue	analogous EPA 350.1, APHA 4500-NH ₃ F, ISO 7150-1, DIN 38406-5	0.5	-	±0.4	1, 6, 8, 11, 13, 16, 18
Indophenol blue	analogous EPA 350.1, APHA 4500-NH ₃ F, ISO 7150-1, DIN 38406-5	0.1 + 0.2 + 5.0	10	±1.7	1, 4, 8, 9, 12, 13, 16, 18
Indophenol blue	analogous EPA 350.1, APHA 4500-NH ₃ F, ISO 7150-1, DIN 38406-5	0.1	-	±1.9	1, 4, 8, 12, 13, 16, 18
Brilliant green	Application, see more information in Prove and NOVA manual	4.0 + 1.0 + 5.0	10	-	11, 18
Iron(III)-thiocyanate	adsorption analogous EN ISO 9562	0.2 + 1.0 + 7.0	-	±0.20	5, 8, 9, 10, 11, 13, 15, 18
-	additionally required for AOX measurement	-	-	-	
-	for multiple use, additionally required for AOX measurement	-	-	-	

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater
5 Boiler water, cooling water			
6 Construction-material industry			

Spectroquant® Test Kits

Parameters A-C

	Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
		Prove 100/300/600	NOVA 30/60	Multy	Move 100			
A	AOX Standard 0.2 – 2.0 mg/L	–	–	–	–	–	8 – 16	1.00680.0001
	Arsenic Test	0.001 – 0.100	0.001 – 0.100 •	5 – 100 µg/L	5 – 100 µg/L	As	30	1.01747.0001
	Arsenic reagent 2: Sulfuric acid 95 – 97 % for analysis EMSURE® ISO	–	–	–	–	–	50	1.00731.1000
	Arsenic reagent 7: Zinc granular for analysis, particle size about 3 – 8 mm EMSURE® ISO	–	–	–	–	–	27	1.08780.0500
	Absorption Tube for Arsenic with ground joint NS29	–	–	–	–	–	1	1.73501.0001
B	BOD Cell Test ^{A)}	0.5 – 3,000	0.5 – 3,000	0.5 – 3,000	0.5 – 3,000	BOD	50	1.00687.0001
	BOD Nutrient Salt Mixture (with allyl thiourea)	–	–	–	–	–	12 L	1.00688.0001
	BOD (Oxygen) Reaction bottle	–	–	–	–	–	1	1.14663.0001
	BOD Standard 210 ±20 mg/L	–	–	–	–	–	10 L	1.00718.0001
	Boron Test	0.050 – 0.800	0.050 – 0.800	–	–	B	60	1.14839.0001
	Boron Cell Test	0.05 – 2.00	0.05 – 2.00	0.05 – 2.00	0.05 – 2.00	B	25	1.00826.0001
	Bromate	0.5 – 100 µg/L ^{D)} 1.0 – 200 µg/L ^{E)}	0.003 – 0.120	–	–	BrO ₃	–	–
	Bromine Test	0.020 – 10.00	0.020 – 10.00	0.10 – 5.00	0.10 – 5.00	Br ₂	200	1.00605.0001
	Cadmium Test ^{C)}	0.0020 – 0.500	0.0020 – 0.500 •	5 – 500 µg/L	5 – 500 µg/L	Cd	55	1.01745.0001
	Cadmium Cell Test ^{C)}	0.025 – 1.000	0.025 – 1.000	25 – 1.000 µg/L	25 – 1.000 µg/L	Cd	25	1.14834.0001
C	Calcium Test	0.20 – 4.00	0.20 – 4.00	–	–	Ca	100	1.00049.0001
	Calcium Test	1.0 – 15.0	1.0 – 15.0	5 – 160	5 – 160	Ca	100	1.14815.0001
		1.4 – 21.0	1.4 – 21.0	7 – 224	7 – 224	CaO		
		2.5 – 37.5	2.5 – 37.5	13 – 400	13 – 400	CaCO ₃		
		5 – 160	5 – 160			Ca		
		7 – 224	7 – 224			CaO		
		12 – 400	12 – 400			CaCO ₃		

A. The cell test contains four 16 mm cells with a bar-code label. After measurement, the cells can be emptied and cleaned for subsequent measurements. | C. For determination of total content of this parameter, use one of the Crack Sets before the photometric procedure, see page 51. | D. With Prove 600. | E. With Prove 100 and 300. | • Only with NOVA 60



BROMATE BONUS

Learn more about hassle-free bromate analysis in our webinar (simply scan the QR code).

And for more information, visit:

www.merckmillipore.com/bromate



www.merckmillipore.com/photometry

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
–	for 8 – 16 quality tests, analogous DIN EN ISO 9562	5.0 / 10.0	–	–	5, 8, 9, 10, 11, 13, 15, 18
Silver DDTC	analogous EPA 206.4, APHA 3500-As B, ASTM D2972-08A	1.0 + 5.0 + 20 (+ 350)	10, 20	±0.003	5, 8, 9, 10, 11, 13, 15, 18
–	additionally required for Arsenic measurement	–	–	–	
–	additionally required for Arsenic measurement	–	–	–	
–	for multiple use, additionally required for Arsenic measurement	–	–	–	
mod. Winkler method	–	–	–	±0.5	2, 8, 9, 10, 11, 13, 16, 18
–	for 12 x 1 L nutrient salt solution, additionally required for BOD measurement, anal. DIN EN 1899	20	–	–	
–	4 bottles are necessary for 1 determination, 6 for 2, 8 for 3 etc.	–	–	–	
–	for 10 x 1 L standard solution, analogous DIN EN 1899	–	–	–	
Rosocyanine	analogous EPA 212.3, ASTM D3082-09, APHA 4500-B B	0.5 + 0.8 + 1.0 + 1.5 + 5.0 + 6.0	10	±0.030	1, 9, 11, 13, 15, 18
Azomethine H	analogous DIN 38405-17	1.0 + 4.0	–	±0.09	1, 9, 11, 13, 15, 16, 18
3,3'- Dimethyl-naphtidine	Application, see more information in Prove and NOVA manual	10 + 0.10 + 0.20	100 50		7, 9, 13, 15
DPD	–	10	10, 20, 50	±0.047	5, 7, 9, 17, 18
Cadion derivative	–	0.2 + 1.0 + 10	10, 20, 50	±0.0039	5, 8, 9, 10, 11, 13, 15, 18
Cadion derivative	–	0.2 + 5.0	–	±0.025	5, 8, 9, 10, 11, 13, 15, 18
Phthalein derivate	–	0.5 + 5.0	10	±0.11	2, 3, 5, 9, 11, 12, 13
Glyoxalbis-hydroxyanil	for determinations in the low measuring range see manual NOVA / Prove	0.5 + 5.0 0.10 + 5.0	10 10, 20	±1.8 ±3	1, 2, 5, 6, 9, 13, 15, 16,

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater
5 Boiler water, cooling water			
6 Construction-material industry			

Spectroquant® Test Kits

Parameters C

Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
	Prove 100/300/600	NOVA 30/60	Multy	Move 100			
C Calcium Cell Test	10 – 250	10 – 250	10 – 250	10 – 250	Ca	25	1.00858.0001
	14 – 350	14 – 350	14 – 350	14 – 350	CaO		
	25 – 624	25 – 624	25 – 625	25 – 625	CaCO ₃		
Carbohydrazide							
Chloride Test	0.10 – 5.00	0.10 – 5.00	0.50 – 5.00	0.50 – 5.00	Cl	100	1.01807.0001
Chloride Cell Test	0.5 – 15.0	0.5 – 15.0	0.5 – 15.0	0.5 – 15.0	Cl	25	1.01804.0001
Chloride Test	2.5 – 250	2.5 – 250 •	10 – 250	10 – 250	Cl	100	1.14897.0001
						175	1.14897.0002
Chloride Cell Test	5 – 125	5 – 125	5 – 125	5 – 125	Cl	25	1.14730.0001
USEPA approved Chlorine Test (free chlorine) ^{B.2)}	0.010 – 6.00	0.010 – 6.00 •	0.02 – 6.00	0.02 – 6.00	Cl ₂	200	1.00598.0002
						1,200	1.00598.0001
USEPA approved Chlorine Cell Test ^{A)} (free chlorine) ^{B.2)}	0.03 – 6.00	0.03 – 6.00	0.05 – 5.00	0.05 – 5.00	Cl ₂	200	1.00595.0001
USEPA approved Chlorine Test (total chlorine) ^{B.3)}	0.010 – 6.00	0.010 – 6.00 •	0.02 – 6.00	0.02 – 6.00	Cl ₂	200	1.00602.0001
						1,200	1.00602.0002
USEPA approved Chlorine Test 100 tests free chlorine + 100 tests chlorine (total) ^{B.3)}	0.010 – 6.00	0.010 – 6.00 •	0.02 – 6.00	0.02 – 6.00	Cl ₂	200	1.00599.0001
USEPA approved Chlorine Cell Test ^{A)} 100 tests free chlorine + 100 tests chlorine (total) ^{B.3)}	0.03 – 6.00	0.03 – 6.00	0.05 – 5.00	0.05 – 5.00	Cl ₂	200	1.00597.0001
Chlorine Reagent Cl ₂ -1 (liquid) ^{F)}	0.03 – 6.00	0.03 – 6.00	0.02 – 6.00	0.02 – 6.00	Cl ₂	200	1.00086.0001
Chlorine Reagent Cl ₂ -2 (liquid) ^{F)}	0.03 – 6.00	0.03 – 6.00	0.02 – 6.00	0.02 – 6.00	Cl ₂	400	1.00087.0001
Chlorine Reagent Cl ₂ -3 (liquid) ^{F)}	0.03 – 6.00	0.03 – 6.00	0.02 – 6.00	0.02 – 6.00	Cl ₂	600	1.00088.0001
Cells and accessories for the photometric chlorine measurement with liquid reagents 1.00086, 1.00087 and 1.00088	–	–	–	–	Cl ₂	25	1.00089.0001
Chlorine Dioxide Test	0.020 – 10.00	0.020 – 10.00 •	0.05 – 10.00	0.05 – 10.00	ClO ₂	200	1.00608.0001
Chlorophyll-a and Phaeophytin-a	–	–	–	–	Chl-a Phaeo	–	–
Chlorophyll-a, -b, -c	–	–	–	–	Chl-a Chl-b Chl-c	–	–

A. The cell test contains four 16 mm cells with a bar-code label. After measurement, the cells can be emptied and cleaned for subsequent measurements. | B. This method is officially recognized by the USEPA as an alternative method for the investigation of 1. wastewater, 2. drinking water 3. drinking water and wastewater. | F. Combination for free or total chlorine, see comment cells and accessories Ord. No. 1.00089.0001. | • Only with NOVA 60



drinking water

Check limits according to WHO, EU and
USEPA regulations on page 56

www.merckmillipore.com/photometry

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
Phthalein complexone	–	0.5 + 1.0	–	±9	1, 2, 5, 6, 9, 13, 15
	see Oxygen Scavengers Test				
Iron(III)-thiocyanate	analogous EPA 325.1, APHA 4500-Cl ⁻ E	0.20 + 10	50	±0.10	2, 5, 6, 9, 12, 13, 15, 18
Iron(III)-thiocyanate	analogous EPA 325.1, APHA 4500-Cl ⁻ E	0.25 + 10	–	±0.3	2, 5, 6, 9, 12, 13, 15, 18
Iron(III)-thiocyanate	analogous EPA 325.1, APHA 4500-Cl ⁻ E	1.0 + 5.0 + 0.5	10	±1.0	1, 2, 5, 6, 8, 9, 10, 12, 13, 15, 16, 18
Iron(III)-thiocyanate	analogous EPA 325.1, APHA 4500-Cl ⁻ E	0.5 + 1.0	–	±5	1, 2, 5, 6, 8, 9, 10, 12, 13, 15, 16, 18
DPD	analogous EPA 330.5, APHA 4500-Cl ₂ G, DIN EN ISO 7393-2	10	10, 20, 50	±0.034	2, 5, 7, 9, 13, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl ₂ G, DIN EN ISO 7393-2	5.0	–	±0.15	2, 5, 7, 9, 13, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl ₂ G, DIN EN ISO 7393-2	10	10, 20, 50	±0.032	2, 5, 7, 9, 13, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl ₂ G, DIN EN ISO 7393-2	10	10, 20, 50	±0.032	2, 5, 7, 9, 13, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl ₂ G, DIN EN ISO 7393-2	5.0	–	±0.11	2, 5, 7, 9, 13, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl ₂ G, DIN EN ISO 7393-2	10	16, 50	±0.036	2, 5, 7, 9, 13, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl ₂ G, DIN EN ISO 7393-2	10	16, 50	±0.036	2, 5, 7, 9, 13, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl ₂ G, DIN EN ISO 7393-2	10	16, 50	±0.036	2, 5, 7, 9, 13, 17, 18
DPD	additionally required for Chlorine Reagent Cl ₂ -1, Cl ₂ -2, Cl ₂ -3 for free chlorine: Cl ₂ -1 and Cl ₂ -2 for total chlorine: Cl ₂ -1, Cl ₂ -2 and Cl ₂ -3 Measuring range of NOVA 30: 0.03 – 6.00 mg/L Cl ₂	–	–	–	
DPD	analogous APHA 4500-ClO ₂ D, DIN 38408-5	10	10, 20, 50	±0.045	5, 7, 9, 15, 17
–	Application on Prove, analogous APHA 10200 H, ASTM D3731-87, DIN 38412, ISO 10260	–	10, 20, 50	–	1, 2, 13
Trichromatic Method	Application on Prove, analogous APHA 10200 H, ASTM D3731-87	–	10, 50	–	1, 2, 13

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater
5 Boiler water, cooling water			
6 Construction-material industry			

Spectroquant® Test Kits

Parameters C

	Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
		Prove 100/300/600	NOVA 30/60	Multy	Move 100			
C	Chromate Test ^C for the determination of chromium (VI)	0.010 – 3.00 0.02 – 6.69	0.010 – 3.00 • 0.02 – 6.69	10 – 1,400 µ/L 22 – 3,123 µ/L	10 – 1,400 µ/L 22 – 3,123 µ/L	Cr CrO ₄	250	1.14758.0001
USEPA approved	Chromate Cell Test for the determination of chromium (VI) and chromium (total) ^{B.1)}	0.05 – 2.00 0.11 – 4.46	0.05 – 2.00 0.11 – 4.46	0.05 – 2.00 0.11 – 4.46	0.05 – 2.00 0.11 – 4.46	Cr CrO ₄	25	1.14552.0001
	Chromium in electroplating baths (inherent color)	4.0 – 400 g/L	4.0 – 400 g/L	–	–	CrO ₃	–	–
USEPA approved	COD Cell Test ^{B.1)}	4.0 – 40.0	4.0 – 40.0	–	–	COD	25	1.14560.0001
USEPA approved	COD Cell Test	5.0 – 80.0	5.0 – 80.0	5.0 – 80.0	5.0 – 80.0	COD	25	1.01796.0001
USEPA approved	COD Cell Test ^{B.1)}	10 – 150	10 – 150	10 – 150	10 – 150	COD	25	1.14540.0001
USEPA approved	COD Cell Test ^{B.1)}	15 – 300	15 – 300	15 – 300	15 – 300	COD	25	1.14895.0001
USEPA approved	COD Cell Test ^{B.1)}	25 – 1,500	25 – 1,500	25 – 1,500	25 – 1,500	COD	25	1.14541.0001
USEPA approved	COD Cell Test ^{B.1)}	50 – 500	50 – 500	50 – 500	50 – 500	COD	25	1.14690.0001
USEPA approved	COD Cell Test ^{B.1)}	300 – 3,500	300 – 3,500	300 – 3,500	300 – 3,500	COD	25	1.14691.0001
USEPA approved	COD Cell Test ^{B.1)}	500 – 10,000	500 – 10,000	500 – 10,000	500 – 10,000	COD	25	1.14555.0001
USEPA approved	COD Cell Test	5,000 – 90,000	5,000 – 90,000	5,000 – 90,000	5,000 – 90,000	COD	25	1.01797.0001
USEPA approved	COD Cell Test for seawater / high chloride contents	5.0 – 60.0	5.0 – 60.0	5.0 – 60.0	5.0 – 60.0	COD	25	1.17058.0001
USEPA approved	COD Cell Test for seawater / high chloride contents	50 – 3,000	50 – 3,000	50 – 3,000	50 – 3,000	COD	25	1.17059.0001
	COD Cell Test for seawater / chloride: Absorption tube	–	–	–	–		1 piece	1.15955.0001
	COD Cell Test for seawater / chloride: Sodalime	–	–	–	–		500 g 2,500 g	1.06733.0501 1.06733.2500
	COD Cell Test for seawater / chloride: Sulfuric Acid for COD determ.	–	–	–	–		1 L	1.17048.1000

B. This method is officially recognized by the USEPA as an alternative method for the investigation of 1. wastewater, 2. drinking water 3. drinking water and wastewater. | C. For determination of total content of this parameter, use one of the Crack Sets before the photometric procedure, see page 51. | • Only with NOVA 60



No Spectroquant® photometer?

To use Spectroquant® test kits with other photometer brands, download our free programming data from:
www.service-test-kits.com

www.merckmillipore.com/photometry

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
Diphenylcarbazide	analogous APHA 3500-Cr B, DIN 38405-24	5.0	10, 20, 50	±0.012	2, 5, 6, 8, 9, 10, 11, 13, 14, 15, 16, 18
Diphenylcarbazide	analogous APHA 3500-Cr B, DIN 38405-24	5.0 (+10)	–	±0.04	2, 5, 6, 8, 10, 11, 13, 14, 16, 18
–	Application, see more information in Prove and NOVA manual	5.0 + 4.0	10, 20, 50	–	10
Oxidation with chromosulfuric acid, determination as chromate	analogous EPA 410.4, APHA 5220 D, ASTM D1252-06B, ISO 15705	3.0	–	±1.5	2, 5, 6, 9, 11, 13, 15, 18
Oxidation with chromosulfuric acid, determination as chromate	analogous EPA 410.4, APHA 5220 D, ASTM D1252-06B, ISO 15705	2.0	–	±1.8	2, 6, 5, 9, 11, 13, 15, 18
Oxidation with chromosulfuric acid, determination as chromate	analogous EPA 410.4, APHA 5220 D, ASTM D1252-06B, ISO 15705	3.0	–	±7	2, 5, 6, 11, 13, 18
Oxidation with chromosulfuric acid, determination as chromate	analogous EPA 410.4, APHA 5220 D, ASTM D1252-06B, ISO 15705	2.0	–	±8	2, 5, 6, 11, 13, 18
Oxidation with chromosulfuric acid, determination as chromium(III)	analogous EPA 410.4, APHA 5220 D, ASTM D1252-06B, ISO 15705	3.0	–	±29	2, 8, 10, 11, 18
Oxidation with chromosulfuric acid, determination as chromate	analogous EPA 410.4, APHA 5220 D, ASTM D1252-06B, ISO 15705	2.0	–	±13	2, 8, 10, 11, 18
Oxidation with chromosulfuric acid, determination as chromium(III)	analogous EPA 410.4, APHA 5220 D, ASTM D1252-06B, ISO 15705	2.0	–	±63	8, 10, 11, 18
Oxidation with chromosulfuric acid, determination as chromium(III)	analogous EPA 410.4, APHA 5220 D, ASTM D1252-06B, ISO 15705	1.0	–	±143	1, 3, 8, 10, 11, 12, 14, 18
Oxidation with chromosulfuric acid, determination as chromium(III)	analogous EPA 410.4, APHA 5220 D, ASTM D1252-06B, ISO 15705	0.1	–	±1,151	1, 3, 8, 10, 11, 12, 14, 16, 18
Oxidation with chromosulfuric acid, determination as chromate	chloride depletion method corresponds to DIN 38409-41-2, method corresponds to DIN ISO 15705, analogous EPA 410.4, APHA 5220 D and ASTM D1252-06 B	20 + 25 + 5.0	–	±3.0	2, 3, 4, 6, 8, 10, 11, 13, 16, 18
Oxidation with chromosulfuric acid, determination as chromium(III)	chloride depletion method corresponds to DIN 38409-41-2, method corresponds to DIN ISO 15705, analogous EPA 410.4, APHA 5220 D and ASTM D1252-06 B	20 + 25 + 3.0	–	±44	2, 3, 4, 6, 8, 10, 11, 13, 16, 18
–	additionally required for COD Cell Test for seawater / high chloride contents	–	–	–	
–	additionally required for COD Cell Test for seawater / high chloride contents	–	–	–	
–	additionally required for COD Cell Test for seawater / high chloride contents	–	–	–	

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater
5 Boiler water, cooling water			
6 Construction-material industry			

Spectroquant® Test Kits

Parameters C

Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
	Prove 100/300/600	NOVA 30/60	Multy	Move 100			
C COD Cell Test (Hg free)	10 – 150	10 – 150	10 – 150	10 – 150	COD	25	1.09772.0001
USEPA approved COD Cell Test (Hg free)	100 – 1,500	100 – 1,500	100 – 1,500	100 – 1,500	COD	25	1.09773.0001
Color, ADMI	2.0 – 500	–	–	–	–	–	–
Color, Hazen	0.2 – 500	0.2 – 500 •	–	–	Pt, Pt/Co, Hazen, CU	–	–
Color, Hazen	0 – 1,000 (at 445, 455, 465 nm)	0 – 1,000 • (at 445 nm)	0 – 1,000 (at 430 nm)	25 – 1,000 (at 430 nm)	Pt, Pt/Co, Hazen, CU	–	–
Color, Spectral Absorption Coefficient	0.1 – 250 m ⁻¹	0.1 – 50.0 m ⁻¹ •	–	–	–	–	–
Color, true color	2 – 2,500	–	–	–	Pt, Pt/Co, CU	–	–
Copper Test C	0.02 – 6.00	0.02 – 6.00 •	0.10 – 6.00	0.10 – 6.00	Cu	250	1.14767.0001
Copper Cell Test C	0.05 – 8.00	0.05 – 8.00	0.05 – 8.00	0.05 – 8.00	Cu	25	1.14553.0001
Copper in electroplating baths (inherent color)	2.0 – 80.0 g/L	2.0 – 80.0 g/L	–	–	Cu	–	–
Cyanide Test (free and readily liberated cyanide)	0.0020 – 0.500	0.0020 – 0.500 •	5 – 200 µg/L	5 – 200 µg/L	CN	100	1.09701.0001
USEPA approved Cyanide Cell Test (free and readily liberated cyanide) B.1)	0.010 – 0.500	0.010 – 0.500	10 – 350 µg/L	10 – 350 µg/L	CN	25	1.14561.0001
Cyanide Cell test (free cyanide)	0.010 – 0.500	0.010 – 0.500	10 – 350 µg/L	10 – 350 µg/L	CN	25	1.02531.0001
Cyanuric Acid Test	2 – 160	2 – 160 •	2 – 160	2 – 160	Cyanuric acid	100	1.19253.0001



cyanide okay?

Need to just check free cyanide in water?
Our cell tests speeds up your time to result with only 2 steps and has fewer reagents, so it lowers your costs and protects the environment.

B. This method is officially recognized by the USEPA as an alternative method for the investigation of 1. wastewater, 2. drinking water 3. drinking water and wastewater. | **C.** For determination of total content of this parameter, use one of the Crack Sets before the photometric procedure, see page 51. | • Only with NOVA 60



more color

Interested in color measurement?
Check our complete range of color methods
on page 48

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
Oxidation with chromosulfuric acid, determination as chromate	–	2.0	–	±8	9, 11, 13, 18
Oxidation with chromosulfuric acid, determination as chromium(III)	–	2.0	–	±32	11, 18
own coloring	physical measurement, analogous to APHA 2120 F	–	10, 50	–	
own coloring	physical measurement, corresponds to APHA 2120 B, DIN EN ISO 6271-2, at 340 nm	–	10, 20, 50	–	
own coloring	physical measurement, corresponds to APHA 2120 B, DIN EN ISO 6271-2	–	50	–	
own coloring	physical measurement according EN ISO 7887, at 445, 525 and 620 nm with NOVA 60, at 436, 525 and 620 nm with Prove 100/300/600	–	10, 20, 50	–	
own coloring	physical measurement according EN ISO 7887, at 410 nm	–	10, 20, 50	–	
Cuprizone	–	5.0	10, 20, 50	±0.034	1, 2, 5, 6, 8, 9, 10, 11, 13, 16, 18
Cuprizone	–	5.0	–	±0.13	1, 2, 5, 6, 8, 9, 10, 11, 13, 16, 18
–	Application, see more information in Prove and NOVA manual	25 + 5.0	10, 20, 50		10
Barbituric acid, pyridine-carboxylic acid	analogous EPA 335.2, APHA 4500-CN ⁻ E, ASTM D2036-09D, ISO 6703, DIN 38405-13	5.0 + 10	10, 20, 50	±0.0025	8, 9, 10, 11, 13, 15, 18
Barbituric acid, pyridine-carboxylic acid	analogous EPA 335.2, APHA 4500-CN ⁻ E, ASTM D2036-09D, ISO 6703, DIN 38405-13	5.0 + 10	–	±0.013	8, 9, 10, 11, 13, 15, 18
Barbituric acid, pyridine-carboxylic acid	analogous EPA 335.2, APHA 4500-CN ⁻ E, ASTM D2036-09D, ISO 6703, DIN 38405-13	5.0	–	±0.013	8, 9, 10, 11, 13, 15, 18
Turbidity	–	5.0	20	±5	7, 11, 17



Analyzing COD

Analyzing COD in water or wastewater?
Our nine COD cell tests cover the entire measuring range from 4.0 to 90,000 mg/L. Get fast, error-free results – without sample dilution.

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
5 Boiler water, cooling water	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
6 Construction-material industry	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater

Spectroquant® Test Kits

Parameters D-L

	Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
		Prove 100/300/600	NOVA 30/60	Multy	Move 100			
D	DEHA (Diethylhydroxylamine)							
	Detergents							
F	Fluoride Cell Test	0.025 - 0.500 0.10 - 1.80	0.025 - 0.500 • 0.10 - 1.80 •	0.10 - 1.80	0.10 - 1.80	F	25	1.00809.0001
	Fluoride Test	0.02 - 2.00	0.02 - 2.00 •	0.08 - 2.00	0.08 - 2.00	F	250	1.00822.0250
	Fluoride Test	0.10 - 20.0	0.10 - 20.0 •	0.10 - 2.00	0.10 - 2.00	F	100 250	1.14598.0001 1.14598.0002
	Formaldehyde Test	0.02 - 8.00	0.02 - 8.00 •	–	–	HCHO	100	1.14678.0001
	Formaldehyde Cell Test	0.10 - 8.00	0.10 - 8.00	–	–	HCHO	25	1.14500.0001
G	Gold Test	0.5 - 12.0	0.5 - 12.0	–	–	Au	75	1.14821.0002
H	Hardness							
	Hazen Color Number (Pt/Co / APHA / Hazen)	0 - 1,000	0 - 1,000	0 - 1,000	25 - 1,000	Pt, Pt/Co, Hazen, CU		
	Hydrazine Test	0.005 - 2.00	0.005 - 2.00 •	10 - 1,200 µ/L	10 - 1,200 µ/L	N ₂ H ₄	100	1.09711.0001
	Hydrogen Peroxide Test	0.015 - 6.00	0.015 - 6.00 •	0.02 - 5.50	0.02 - 5.50	H ₂ O ₂	100	1.18789.0001
	Hydrogen Peroxide Cell Test	2.0 - 20.0 0.25 - 5.00	2.0 - 20.0 • 0.25 - 5.00 •	–	–	H ₂ O ₂ H ₂ O ₂	25	1.14731.0001
	Hydrogen sulfide							
	Hydroquinone							
I	Iodine color number	0.010 - 50.0	0.010 - 50.0 •	–	–	IFZ	–	
	Iodine Test	0.050 - 10.00	0.050 - 10.00	0.10 - 5.00	0.10 - 5.00	I ₂	200	1.00606.0001
	Iron Test ^{C)}	0.0005 - 0.0100 ^{D)} 0.0025 - 5.00 ^{D)} 0.005 - 5.00	0.005 - 5.00 •	0.01 - 2.00	0.01 - 2.00	Fe	250 1,000	1.14761.0002 1.14761.0001
	Iron Test ^{C)}	0.010 - 5.00	0.010 - 5.00 •	0.10 - 5.00	0.10 - 5.00	Fe	150	1.00796.0001
	Iron Cell Test ^{C)}	0.05 - 4.00	0.05 - 4.00	0.05 - 4.00	0.05 - 4.00	Fe	25	1.14549.0001
	Iron Cell Test ^{C)}	1.0 - 50.0	1.0 - 50.0	–	–	Fe	25	1.14896.0001
	Isoascorbic acid (erythorbic acid)							
L	Lead Test ^{C)}	0.010 - 5.00	0.010 - 5.00 •	0.05 - 5.00	0.05 - 5.00	Pb	50	1.09717.0001
	Lead Cell Test ^{C)}	0.10 - 5.00	0.10 - 5.00	0.10 - 5.00	0.10 - 5.00	Pb	25	1.14833.0001

C. For determination of total content of this parameter, use one of the Crack Sets before the photometric procedure, see page 51. | D. With Prove 600. | • Only with NOVA 60

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
	see Oxygen Scavengers Test				
	see Surfactants				
Alizarin complexone	analogous EPA 340.3, APHA 4500-F ⁻ E for determinations in the low measuring range see manual NOVA / Prove	10 5.0	50 –	±0.024 ±0.06	9, 10, 11, 13, 15, 18
SPADNS method	analogous to APHA 4500-F ⁻ D	5.0 + 1.0	50	±0.04	8, 9, 10, 11, 13, 15, 16, 18
Alizarin complexone	analogous EPA 340.3, APHA 4500-F ⁻ E	0.5 + 2.0 + 5.0	10	±0.12	9, 10, 11, 13, 15, 16, 18
Chromotropic acid	–	3.0 + 4.5	10, 20, 50	±0.03	7, 9, 10, 11, 15, 18
Chromotropic acid	–	2.0	–	±0.18	7, 9, 10, 11, 15, 18
Rhodamine B	–	2.0 + 6.0	10	±0.4	10, 13, 16,
	see Total Hardness or Residual Hardness				
own coloring	see Color, Hazen	–	10, 20, 50	–	5, 9, 10, 11, 12, 13, 15, 18
4-(Dimethylamino)-benzaldehyde	analogous DIN 38413-1	2.0 + 5.0	10, 20, 50	±0.007	5
Neocuproin	–	8.0 + 0.5	10, 20	±0.033	3, 7, 9, 11, 12, 13, 14, 15
Titanyl sulfate	analogous DIN 38409-15 for determinations in the low measuring range see manual of instrument	10 10	– 50	±0.9	3, 7, 9, 11, 12, 13, 14, 15, 18
	see Sulfide				
	see Oxygen Scavengers Test				
own coloring	corresponds to DIN 6162 A	–	10, 20, 50	–	3, 11, 12
DPD	–	10	10, 20, 50	±0.060	7, 9, 17
Triazine	–	5.0	100 100 10, 20, 50	±0.014	1, 2, 5, 6, 8, 9, 10, 11, 12, 13, 15, 16, 17, 18
1,10-Phenanthroline	differentiation between Fe(II) and Fe(III) possible, analogous APHA 3500-Fe B, DIN 38406-1	0.5 + 8.0	10, 20, 50	±0.024	1, 2, 5, 6, 8, 9, 10, 11, 12, 13, 15, 16, 17, 18
Triazine	–	5.0	–	±0.06	1, 2, 6, 8, 9, 10, 11, 12, 13, 15, 16, 18
2,2'-Bipyridine	differentiation between Fe(II) and Fe(III) possible	1.0	–	±0.9	6, 8, 10, 11, 13, 18
	see Oxygen Scavengers Test				
PAR	–	0.5 + 8.0	10, 20, 50	±0.028	2, 5, 8, 9, 10, 11, 15, 18
PAR	–	5.0	–	±0.08	1, 2, 6, 9, 10, 12, 13, 15, 18

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater

Spectroquant® Test Kits

Parameters M-N

	Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
		Prove 100/300/600	NOVA 30/60	Multy	Move 100			
M	Magnesium Cell Test	5.0 – 75.0	5.0 – 75.0	5.0 – 75.0	5.0 – 75.0	Mg	25	1.00815.0001
	Manganese Test	0.005 – 2.00	0.005 – 2.00 •	0.05 – 1.80	0.05 – 1.80	Mn	250	1.01846.0001
	Manganese Test	0.010 – 10.00	0.010 – 10.00 •	0.05 – 6.00	0.05 – 6.00	Mn	250 500	1.14770.0002 1.14770.0001
	Manganese Cell Test	0.10 – 5.00	0.10 – 5.00	0.10 – 5.00	0.10 – 5.00	Mn	25	1.00816.0001
	Mercury	0.025 – 1.000	0.025 – 1.000	–	–	Hg	–	–
	Methylethylketoxime (2-Butanoneoxime)							
	Molybdenum Cell Test	0.02 – 1.00 0.03 – 1.67 0.04 – 2.15	0.02 – 1.00 • 0.03 – 1.67 • 0.04 – 2.15 •	0.02 – 1.00 0.03 – 1.67 0.04 – 2.15	0.02 – 1.00 0.03 – 1.67 0.04 – 2.15	Mo MoO ₄ ²⁺ Na ₂ MoO ₄	25	1.00860.0001
	Monochloramine Test	0.050 – 10.00 0.036 – 7.26 0.010 – 1.98	0.050 – 10.00 • 0.036 – 7.26 • 0.010 – 1.98 •	0.10 – 5.00 0.07 – 3.63 0.02 – 0.99	0.10 – 5.00 0.07 – 3.63 0.02 – 0.99	Cl ₂ NH ₂ Cl NH ₂ Cl-N	150	1.01632.0001
	Nickel Test ^{C)}	0.02 – 5.00	0.02 – 5.00 •	0.05 – 5.00	0.05 – 5.00	Ni	250	1.14785.0001
	Nickel Cell Test ^{C)}	0.10 – 6.00	0.10 – 6.00	0.10 – 6.00	0.10 – 6.00	Ni	25	1.14554.0001
USEPA approved	Nickel in electroplating baths (inherent color)	2.0 – 120 g/L	2.0 – 120 g/L	–	–	Ni	–	–
	Nitrate (UV)	0.0 – 7.0	–	–	–	NO ₃ -N	–	–
	Nitrate Test ^{B,3)} ^{C)}	0.10 – 25.0	0.10 – 25.0 •	–	–	NO ₃ -N	100	1.09713.0001
		0.4 – 110.7	0.4 – 110.7 •	–	–	NO ₃	250	1.09713.0002
	Nitrate Test ^{B,3)} ^{C)}	0.2 – 20.0	0.2 – 20.0 •	0.5 – 15.0	0.5 – 15.0	NO ₃ -N	100	1.14773.0001
		0.89 – 88.5	0.89 – 88.5 •	2.2 – 66.4	2.2 – 66.4	NO ₃		
	Nitrate Test ^{B,3)} ^{C)}	0.3 – 30.0	0.3 – 30.0 •	0.3 – 30.0	0.3 – 30.0	NO ₃ -N	100	1.01842.0001
		1.3 – 132.8	1.3 – 132.8 •	1.3 – 132.8	1.3 – 132.8	NO ₃		
	Nitrate Cell Test ^{B,3)} ^{C)}	0.5 – 18.0	0.5 – 18.0	0.5 – 15.0	0.5 – 15.0	NO ₃ -N	25	1.14542.0001
		2.2 – 79.7	2.2 – 79.7	2.2 – 66.4	2.2 – 66.4	NO ₃		
	Nitrate Cell Test ^{B,3)} ^{C)}	0.5 – 25.0	0.5 – 25.0	–	–	NO ₃ -N	25	1.14563.0001
		2.2 – 110.7	2.2 – 110.7	–	–	NO ₃		
	Nitrate Cell Test ^{B,3)} ^{C)}	1.0 – 50.0	1.0 – 50.0	–	–	NO ₃ -N	25	1.14764.0001
		4 – 221	4 – 221	–	–	NO ₃		
	Nitrate Cell Test ^{B,3)}	23 – 225	23 – 225	–	–	NO ₃ -N	25	1.00614.0001
		102 – 996	102 – 996	–	–	NO ₃		

B. This method is officially recognized by the USEPA as an alternative method for the investigation of 1. wastewater, 2. drinking water 3. drinking water and wastewater. | C. For determination of total content of this parameter, use one of the Crack Sets before the photometric procedure, see page 51. | • Only with NOVA 60



ANALYTICAL APPLICATION NOTES FINDER

Struggling with sample preparation for nitrate analysis in soil? Check our application notes on www.merckmillipore.com/aaf > [Photometry](#)

www.merckmillipore.com/photometry

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
Phthalein complexone	–	1.0	–	±4.0	1, 2, 9, 10, 15, 18
PAN	–	8.0 + 2.0 + 0.25	10, 20, 50	±0.007	1, 2, 9, 10, 13, 15
Formaldioxime	analogous DIN 38406-2	5.0	10, 20, 50	±0.035	1, 2, 9, 10, 13, 15, 18
Formaldioxime	analogous DIN 38406-2	7.0	–	±0.08	1, 2, 10, 13, 18
Michler's thioketone	Application, see more information in Prove and NOVA manual	2.5 + 5.0 + 1.0 + 1.5	50	–	11, 18
see Oxygen Scavengers Test					
Bromopyrogallol red	–	10	–	±0.04	1, 5, 9, 13, 15, 18
Indophenol blue	–	0.6 + 10	10, 20, 50	±0.033	7, 9, 17
Dimethylglyoxime	–	5.0	10, 20, 50	±0.03	3, 5, 8, 9, 10, 11, 13, 15, 18
Dimethylglyoxime	–	5.0	–	±0.11	3, 5, 8, 10, 11, 18
–	Application, see more information in Prove and NOVA manual	5.0	10, 20, 50	–	10
direct measurement in the UV range	Application on Prove 300, analogous to APHA 4500-NO ₃ ⁻ B, quartz cuvette required	50 + 1.0	10	–	9, 13
2,6-Dimethylphenol	analogous DIN 38405-9	0.5 + 4.0	10, 20, 50	±0.11	2, 6, 8, 9, 11, 13, 15, 17, 18
Nitrospectral	–	1.5 + 5.0	10, 20	±0.31	2, 6, 9, 11, 13, 15, 17, 18
Cadmium Reduction	–	10	50	±1.2	1, 2, 6, 8, 9, 10, 11, 13, 15, 17, 18
Nitrospectral	–	1.5	–	±0.5	1, 2, 6, 8, 9, 11, 13, 15, 17, 18
2,6-Dimethylphenol	analogous DIN 38405-9	1.0	–	±0.5	1, 2, 6, 9, 11, 13, 15, 17, 18
2,6-Dimethylphenol	analogous DIN 38405-9	0.5 + 1.0	–	±1.0	1, 2, 8, 9, 11, 13, 15, 18
2,6-Dimethylphenol	analogous DIN 38405-9	0.1 + 1.0	–	±5.0	1, 8, 11, 13, 18

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater
5 Boiler water, cooling water			
6 Construction-material industry			

Spectroquant® Test Kits

Parameters N-P

	Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
		Prove 100/300/600	NOVA 30/60	Multy	Move 100			
N	Nitrate Cell Test in seawater	0.10 – 3.00	0.10 – 3.00 •	0.10 – 3.00	0.10 – 3.00	NO ₃ -N	25	1.14556.0001
		0.4 – 13.3	0.4 – 13.3 •	0.4 – 13.3	0.4 – 13.3	NO ₃		
	Nitrate Test in seawater	0.2 – 17.0	0.2 – 17.0 •	–	–	NO ₃ -N	50	1.14942.0001
		0.9 – 75.3	0.9 – 75.3 •			NO ₃		
	Nitrite Test ^{B.3)}	0.002 – 1.00	0.002 – 1.00 •	5 – 400 µg/L	5 – 400 µg/L	NO ₂ -N	335	1.14776.0002
		0.007 – 3.28	0.007 – 3.28 •	16 – 1,313 µg/L	16 – 1,313 µg/L	NO ₂	1,000	1.14776.0001
	Nitrite Cell Test ^{B.3)}	0.010 – 0.700	0.010 – 0.700	10 – 700 µg/L	10 – 700 µg/L	NO ₂ -N	25	1.14547.0001
		0.03 – 2.30	0.03 – 2.30	33 – 2,299 µg/L	33 – 2,299 µg/L	NO ₂		
	Nitrite Cell Test ^{B.3)}	1.0 – 90.0	1.0 – 90.0	1.0 – 90.0	1.0 – 90.0	NO ₂ -N	25	1.00609.0001
		3.0 – 295.2	3.3 – 295.2	3.3 – 295.2	3.3 – 295.2	NO ₂		
O	Nitrogen (total) Cell Test	0.5 – 15.0	0.5 – 15.0	–	–	N	25	1.00613.0001
	Nitrogen (total) Cell Test	0.5 – 15.0	0.5 – 15.0	0.5 – 15.0	0.5 – 15.0	N	25	1.14537.0001
	Nitrogen (total) Cell Test	10 – 150	10 – 150	–	–	N	25	1.14763.0001
	Organic Carbon, Total							
	Oxygen Cell Test	0.5 – 12.0	0.5 – 12.0	0.5 – 12.0	0.5 – 12.0	O ₂	25	1.14694.0001
	Oxygen Demand, Biological							
	Oxygen Demand, Chemical							
	Oxygen Scavengers Test	0.020 – 0.500	0.020 – 0.500 •	0.020 – 0.500	0.020 – 0.500	DEHA	200	1.19251.0001
		0.027 – 0.667	0.027 – 0.667 •	0.027 – 0.667	0.027 – 0.667	Carbohy		
		0.05 – 1.32	0.05 – 1.32 •	0.053 – 1.315	0.053 – 1.315	Hydro		
P		0.08 – 1.95	0.08 – 1.95 •	0.078 – 1.950	0.078 – 1.950	ISA		
		0.09 – 2.17	0.09 – 2.17 •	0.087 – 2.170	0.087 – 2.170	MEKO		
	Ozone Test	0.010 – 4.00	0.010 – 4.00 •	0.02 – 4.00	0.02 – 4.00	O ₃	200	1.00607.0001
							1,200	1.00607.0002
	Palladium	0.05 – 1.25	0.05 – 1.25 •	–	–	Pd	–	–
	Peroxide							
	pH Cell Test ^{A)}	pH 6.4 – 8.8	pH 6.4 – 8.8	pH 6.4 – 8.8	pH 6.4 – 8.8	pH	280	1.01744.0001
	Phaeophytin-a and Chlorophyll-a							
	Phenol Test	0.002 – 0.100	0.002 – 0.100 •	0.10 – 5.00	0.10 – 5.00	Phenol	50 –	1.00856.0001
		0.025 – 5.00	0.025 – 5.00 •				250	
USEPA approved	Phenol Cell Test	0.10 – 2.50	0.10 – 2.50 •	0.10 – 2.50	0.10 – 2.50	Phenol	25	1.14551.0001
	Phosphate Test ^{C)}	0.0025 – 5.00	0.010 – 5.00 •	0.01 – 2.50	0.01 – 2.50	PO ₄ -P	220	1.14848.0002
	(ortho-phosphate)	0.0077 – 15.30	0.03 – 15.3 •	0.03 – 7.66	0.03 – 7.66	PO ₄	420	1.14848.0001
		0.0057 – 11.46	0.02 – 11.46 •	0.02 – 5.73	0.02 – 5.73	P ₂ O ₅		
		0.0005 – 0.0250 ^{D)}				PO ₄ -P		
		0.0015 – 0.0767 ^{D)}				PO ₄		
		0.0007 – 0.0335 ^{D)}				P ₂ O ₅		
	Phosphate Cell Test	0.05 – 5.00	0.05 – 5.00	0.05 – 4.00	0.05 – 4.00	PO ₄ -P	25	1.00474.0001
	(ortho-phosphate)	0.2 – 15.3	0.2 – 15.3	0.15 – 12.26	0.15 – 12.26	PO ₄		
		0.11 – 11.46	0.11 – 11.46	0.11 – 9.17	0.11 – 9.17	P ₂ O ₅		

A. The cell test contains three 16 mm cells with a bar-code label. After measurement, the cells can be emptied and cleaned for subsequent measurements. | B. This method is officially recognized by the USEPA as an alternative method for the investigation of 1. wastewater, 2. drinking water 3. drinking water and wastewater. | C. For determination of total content of this parameter, use one of the Crack Sets before the photometric procedure, see page 51. | D. With Prove 600. | • Only with NOVA 60



PHOSPHATE AID

Need help with phosphate or phosphonate analysis? Scan the QR code to learn more.



www.merckmillipore.com/photometry

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
Resorcinol	–	2.0	–	±0.09	1, 2, 8, 9, 11, 13, 15, 16, 18
Resorcinol	–	1.0 + 1.5 + 5.0	10	±0.4	1, 2, 8, 9, 11, 13, 15, 16, 18
Griess' reaction	analogous EPA 354.1, APHA 4500-NO ₂ ⁻ B, DIN EN 26777	5.0	10, 20, 50	±0.005	2, 5, 8, 9, 10, 11, 13, 15, 16, 18
Griess' reaction	analogous EPA 354.1, APHA 4500-NO ₂ ⁻ B, DIN EN 26777	5.0	–	±0.010	2, 5, 8, 9, 10, 11, 13, 15, 16, 18
Iron sulfate	–	8.0	–	±2.6	5, 10, 13, 16, 18
Koroleff digestion, 2,6-dimethylphenol	digestion analogous DIN EN ISO 11905-1, determination analogous DIN 38405-9	1.0 + 10	–	±0.5	1, 2, 5, 8, 11, 13, 14, 18
Koroleff digestion, nitrospectral	digestion analogous to DIN EN ISO 11905-1	1.5 + 10	–	±0.6	1, 2, 5, 8, 11, 13, 14, 18
Koroleff digestion, 2,6-dimethylphenol	digestion analogous DIN EN ISO 11905-1, determination analogous DIN 38405-9	1.0 + 9.0	–	±5.0	1, 8, 11, 14, 18
	see TOC				
mod. Winkler method	analogous DIN EN 25813-21	–	–	±0.3	2, 5, 11, 13, 17
	see BOD				
	see COD				
Iron reduction	–	0.2 + 10	20	±0.022	5
DPD	analogous DIN 38408-3	10	10, 20, 50	±0.023	7, 9, 15, 17
Michlers' thioketone	Application, see more information in Prove and NOVA manual	5.0 + 1.0 + 0.20	10	–	10, 18
	see Hydrogen Peroxide				
Indicator	–	10	–	±0.1 pH	2, 5, 7, 9, 13, 15, 16, 17
	see Chlorophyll-a and Phaeophytin-a				1, 2, 13
4-Aminoantipyrine	analogous EPA 420.1, ASTM D1783-01, APHA 5530 C + D, ISO 6439	5.0 + 10 1.0 + 10	20 10, 20, 50	±0.004 ±0.027	8, 9, 11, 13, 16, 18
MBTH		10	–	±0.11	8, 11, 13, 16, 18
Phosphomolybdenum blue	analogous EPA 365.2+3, APHA 4500-P E, DIN EN ISO 6878	5.0	10, 20, 50 100	±0.015	1, 2, 5, 9, 11, 13, 15, 16, 18
Phosphomolybdenum blue	analogous EPA 365.2+3, APHA 4500-P E, DIN EN ISO 6878	5.0	–	±0.08	1, 2, 5, 9, 11, 13, 15, 16, 18

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater
5 Boiler water, cooling water			
6 Construction-material industry			

Spectroquant® Test Kits

Parameters P-S

	Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
		Prove 100/300/600	NOVA 30/60	Multy	Move 100			
P	Phosphate Cell Test (ortho-phosphate and total phosphorus) ^{B,3)}	0.05 – 5.00	0.05 – 5.00	0.05 – 4.00	0.05 – 4.00	PO ₄ -P	25	1.14543.0001
		0.2 – 15.3	0.2 – 15.3	0.15 – 12.26	0.15 – 12.26	PO ₄		
		0.11 – 11.46	0.11 – 11.46	0.11 – 9.17	0.11 – 9.17	P ₂ O ₅		
USEPA approved	Phosphate Cell Test (ortho-phosphate)	0.5 – 25.0	0.5 – 25.0	0.5 – 20.0	0.5 – 20.0	PO ₄ -P	25	1.00475.0001
USEPA approved		1.5 – 76.7	1.5 – 76.7	1.5 – 61.3	1.5 – 61.3	PO ₄		
USEPA approved		1.1 – 57.3	1.1 – 57.3	1.1 – 45.8	1.1 – 45.8	P ₂ O ₅		
USEPA approved	Phosphate Cell Test (ortho-phosphate and total phosphorus) ^{B,3)}	0.5 – 25.0	0.5 – 25.0	0.5 – 20.0	0.5 – 20.0	PO ₄ -P	25	1.14729.0001
		1.5 – 76.7	1.5 – 76.7	1.5 – 61.3	1.5 – 61.3	PO ₄		
		1.1 – 57.3	1.1 – 57.3	1.1 – 45.8	1.1 – 45.8	P ₂ O ₅		
USEPA approved	Phosphate Cell Test (ortho-phosphate)	0.5 – 25.0	0.5 – 25.0	0.5 – 25.0	0.5 – 25.0	PO ₄ -P	25	1.14546.0001
		1.5 – 76.7	1.5 – 76.7	1.5 – 76.7	1.5 – 76.7	PO ₄		
		1.1 – 57.3	1.1 – 57.3	1.1 – 57.3	1.1 – 57.3	P ₂ O ₅		
USEPA approved	Phosphate Test (ortho-phosphate)	0.5 – 30.0	0.5 – 30.0 •	0.5 – 30.0	0.5 – 30.0	PO ₄ -P	400	1.14842.0001
		1.5 – 92.0	1.5 – 92.0 •	1.5 – 92.0	1.5 – 92.0	PO ₄		
		1.1 – 68.7	1.1 – 68.7 •	1.1 – 68.7	1.1 – 68.7	P ₂ O ₅		
USEPA approved	Phosphate Test (ortho-phosphate)	1.0 – 100.0	1.0 – 100.0 •	1.0 – 60.0	1.0 – 60.0	PO ₄ -P	100	1.00798.0001
		3 – 307	3 – 307 •	3.1 – 184	3.1 – 184	PO ₄		
		2 – 229	2 – 229 •	2.3 – 137.5	2.3 – 137.5	P ₂ O ₅		
USEPA approved	Phosphate Cell Test (ortho-phosphate)	3.0 – 100.0	3.0 – 100.0	3.0 – 100.0	3.0 – 100.0	PO ₄ -P	25	1.00616.0001
		9 – 307	9 – 307	9 – 307	9 – 307	PO ₄		
		7 – 229	7 – 229	7 – 229	7 – 229	P ₂ O ₅		
USEPA approved	Phosphate Cell Test (ortho-phosphate and total phosphorus)	3.0 – 100.0	3.0 – 100.0	3.0 – 100.0	3.0 – 100.0	PO ₄ -P	25	1.00673.0001
		9 – 307	9 – 307	9 – 307	9 – 307	PO ₄		
		7 – 229	7 – 229	7 – 229	7 – 229	P ₂ O ₅		
	Platinum	0.10 – 1.25	0.10 – 1.25 •	-	-	Pt	-	-
Platinum-Cobalt Standard								
Method								
	Potassium Cell Test	5.0 – 50.0	5.0 – 50.0	5.0 – 50.0	5.0 – 50.0	K	25	1.14562.0001
	Potassium Cell Test	30 – 300	30 – 300	30 – 300	30 – 300	K	25	1.00615.0001
	Protein Test	0.01 – 1.4 g/L	0.01 – 1.4 g/L	-	-	Protein	200	1.10306.0500
	Protein Test	0.5 – 10 g/L	0.5 – 10 g/L	-	-	Protein	250	1.10307.0500
R	Residual Hardness Cell Test	0.50 – 5.00	0.50 – 5.00	0.50 – 5.00	0.50 – 5.00	Ca	25	1.14683.0001
		0.070 – 0.700	0.070 – 0.700	0.070 – 0.700	0.070 – 0.700	°d		
		0.087 – 0.874	0.087 – 0.874	0.087 – 0.874	0.087 – 0.874	°e		
		0.12 – 1.25	0.12 – 1.25	0.12 – 1.25	0.12 – 1.25	°f		
		0.70 – 7.00	0.70 – 7.00	0.70 – 7.00	0.70 – 7.00	CaO		
		1.2 – 12.5	1.2 – 12.5	1.2 – 12.5	1.2 – 12.5	CaCO ₃		
S	SAC (Spectral absorption coefficient)	0.5 – 250 m ⁻¹	-	-	-	-	-	-

B. This method is officially recognized by the USEPA as an alternative method for the investigation of 1. wastewater; 2. drinking water 3. drinking water and wastewater. | • Only with NOVA 60



Waste disposal advice

Learn how to safely dispose of old test kits:
www.disposal-test-kits.com

www.merckmillipore.com/photometry

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
Phosphomolybdenum blue	analogous EPA 365.2+3, APHA 4500-P E, DIN EN ISO 6878	5.0	–	±0.06	1, 2, 5, 9, 11, 13, 15, 16, 18
Phosphomolybdenum blue	analogous EPA 365.2+3, APHA 4500-P E, DIN EN ISO 6878	1.0	–	±0.5	1, 2, 4, 8, 11, 13, 16, 18
Phosphomolybdenum blue	analogous EPA 365.2+3, APHA 4500-P E, DIN EN ISO 6878	1.0	–	±0.4	1, 2, 4, 8, 11, 13, 16, 18
Vanadato-molybdate	analogous APHA 4500-P C	5.0	–	±0.4	5, 16
Vanadato-molybdate	analogous APHA 4500-P C	1.2 + 5.0	10, 20	±0.2	5, 16
Phosphomolybdenum blue	analogous EPA 365.2+3, APHA 4500-P E, DIN EN ISO 6878	0.5 + 8.0	10	±1.4	1, 2, 4, 8, 11, 12, 13, 18
Phosphomolybdenum blue	analogous EPA 365.2+3, APHA 4500-P E, DIN EN ISO 6878	0.2	–	±1.2	1, 4, 8, 11, 13, 16, 18
Phosphomolybdenum blue	analogous EPA 365.2+3, APHA 4500-P E, DIN EN ISO 6878	0.2	–	±1.4	1, 4, 8, 11, 13, 16, 18
–	Application, see more information in Prove and NOVA manual see Color	5.0 + 1.0 + 0.50	10	–	10, 18
Kalignost®, turbidimetric	–	2.0	–	±2.2	9, 12, 13, 15, 16
Kalignost®, turbidimetric	–	0.5	–	±13	1, 16
Bradford Method	Method not programmed in the photometers	–	10	–	
Biuret Method	Method not programmed in the photometers	–	10	–	
Phthalein complexone	–	0.2 + 4.0	–	±0.14	2, 5, 9
–	physical measurement according DIN 38404, at 436 nm (Prove 100) and 254 + 436 nm (Prove 300)	–	10, 20, 50	–	9, 15

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater
5 Boiler water, cooling water			
6 Construction-material industry			

Spectroquant® Test Kits

Parameters S

	Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
		Prove 100/300/600	NOVA 30/60	Multy	Move 100			
S	Silicate (Silicic Acid) Test	0.00025 – 0.50000 0.00012 – 0.23370 0.00025 – 0.02500 ^{B)} 0.00012 – 0.01168 ^{B)}	0.0005 – 0.5000 • 0.0002 – 0.2337 •	0.004 – 0.500 0.002 – 0.234	0.004 – 0.500 0.002 – 0.234	SiO ₂ Si SiO ₂ Si	100 900	1.01813.0001 1.01813.0002
	Silicate (Silicic Acid) Test	0.011 – 10.70 0.005 – 5.00	0.011 – 10.70 • 0.005 – 5.00 •	0.11 – 8.56 0.05 – 4.00	0.11 – 8.56 0.05 – 4.00	SiO ₂ Si	300	1.14794.0001
	Silicate (Silicic Acid) Test	1.1 – 1,070 0.5 – 500	1.1 – 1,070 • 0.5 – 500 •	11 – 1,070 5 – 500	11 – 1,070 5 – 500	SiO ₂ Si	100	1.00857.0001
	Silver Test	0.25 – 3.00	0.25 – 3.00 •	–	–	Ag	100	1.14831.0001
	Sodium Cell Test in nutrient solutions for fertilization	10 – 300	10 – 300	10 – 300	10 – 300	Na	25	1.00885.0001
	Spectral Absorption Coefficient, Color	0.1 – 250 m ⁻¹	–	–	–	–	–	–
	Spectral Attenuation Coefficient	0.5 – 250 m ⁻¹	–	–	–	–	–	–
	Sulfate Test	0.50 – 50.0	0.50 – 50.0 •	1.0 – 25.0	1.0 – 25.0	SO ₄	100	1.01812.0001
	Sulfate Cell Test	1.0 – 50.0	1.0 – 50.0	2.0 – 50.0	2.0 – 50.0	SO ₄	25	1.02532.0001
	Sulfate Cell Test ^{B.1)}	5 – 250	5 – 250	5 – 250	5 – 250	SO ₄	25	1.14548.0001
USEPA approved	Sulfate Test	5 – 300	5 – 300 •	5 – 300	10 – 300	SO ₄	100 1,000	1.02537.0001 1.02537.0002
	Sulfate Test	25 – 300	25 – 300 •	–	–	–	200	1.14791.0001
	Sulfate Cell Test	50 – 500	50 – 500	50 – 500	50 – 500	SO ₄	25	1.00617.0001
	Sulfate Cell Test ^{B.1)}	100 – 1,000	100 – 1,000	100 – 1,000	100 – 1,000	SO ₄	25	1.14564.0001
	Sulfide Test	0.020 – 1.50	0.020 – 1.50 •	0.10 – 1.50	0.10 – 1.50	S ²⁻	220	1.14779.0001
	Sulfite Cell Test	0.8 – 16.00 1.0 – 20.00 0.05 – 3.00 0.04 – 2.40	0.8 – 16.00 • 1.0 – 20.00 • 0.05 – 3.00 • 0.04 – 2.40 •	1.0 – 20.0	1.0 – 20.0	SO ₂ SO ₃ SO ₃ SO ₂	25	1.14394.0001
	Sulfite Test	1.0 – 60.0 0.8 – 48.0	1.0 – 60.0 • 0.8 – 48.0 •	1.0 – 60.0	1.0 – 60.0	SO ₃ SO ₂	150	1.01746.0001
	Surfactants (anionic) Cell Test	0.05 – 2.00	0.05 – 2.00 •	0.05 – 2.00	0.10 – 2.00	MBAS	25	1.02552.0001
	Surfactants (cationic) Cell Test	0.05 – 1.50	0.05 – 1.50 •	0.05 – 1.50	–	CTAB	25	1.01764.0001
	Surfactants (nonionic) Cell Test	0.10 – 7.50	0.10 – 7.50	0.10 – 7.50	0.10 – 7.50	Triton® X-100	25	1.01787.0001
	Suspended solids	25 – 750	25 – 750	50 – 750	50 – 750	susp. solids	–	–

B. This method is officially recognized by the USEPA as an alternative method for the investigation of 1. wastewater, 2. drinking water 3. drinking water and wastewater. | D. With Prove 600. | • Only with NOVA 60

HIGHER SENSITIVITY

New cell test for anionic surfactants:
now with even higher sensitivity!



www.merckmillipore.com/photometry

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
Silicomolybdenum blue	analogous APHA 4500-SiO ₂ D+E, ASTM D859-10, DIN 38405-21	10 + 0.5	50 100	±0.00449	5, 9, 13, 15
Silicomolybdenum blue	analogous APHA 4500-SiO ₂ D+E, ASTM D859-10, DIN 38405-21	5.0 + 0.5	10, 20, 50	±0.024	5, 6, 9, 13, 16
Molybdosilicate	analogous APHA 4500-SiO ₂ C	0.5 + 2.0 + 4.0 + 5.0	10	±2.1	5, 6, 9, 13, 15
Eosine, 1,10-phenanthroline	reagents for the digestion in the thermoreactor are included in the test kit	1.0 + 10	10, 20	±0.07	10, 18
Iron(III)-thiocyanate	determination as chloride	0.5	–	±13	1
–	see Color, Spectral Absorption Coefficient	–	–	–	
–	physical measurement according DIN 38404, at 254 nm	–	10, 20, 50	–	
Barium sulfate, turbidimetric	analogous EPA 375.4, APHA 4500-SO ₄ ²⁻ E, ASTM D516-11	0.5 + 10	10, 20, 50	±0.90	1, 2, 6, 9, 11, 13, 15, 18
Barium sulfate, turbidimetric	analogous EPA 375.4, APHA 4500-SO ₄ ²⁻ E, ASTM D516-11	10	–	±1.1	1, 6, 9, 11, 13, 15, 18
Barium sulfate, turbidimetric	analogous EPA 375.4, APHA 4500-SO ₄ ²⁻ E, ASTM D516-11	5.0	–	±8	1, 6, 9, 11, 13, 15, 16
Barium sulfate, turbidimetric	analogous EPA 375.4, APHA 4500-SO ₄ ²⁻ E, ASTM D516-11	0.5 + 5	10	±7	1, 6, 9, 11, 13, 15, 16, 18
Tannic acid	–	2.5	10	±14	6, 9, 11, 13, 15
Barium sulfate, turbidimetric	analogous EPA 375.4, APHA 4500-SO ₄ ²⁻ E, ASTM D516-11	2.0 + 5.0	–	±16	1, 6, 9, 11, 13, 15, 16
Barium sulfate, turbidimetric	analogous EPA 375.4, APHA 4500-SO ₄ ²⁻ E, ASTM D516-11	1.0 + 5.0	–	±33	1, 4, 6, 8, 9, 11, 13, 15, 16, 18
Dimethyl-p-phenylenediamine	analogous EPA 376.2, APHA 4500-S ²⁻ D, ISO 10530, DIN 38405-26	5.0	10, 20, 50	±0.017	2, 8, 9, 11, 13, 15, 18
Ellman's reagent	for determinations of the low measuring range see manual NOVA / Prove	3.0 + 7.0	– – 50 50	±0.4	1, 3, 5, 12, 15, 18
Ellman's reagent	–	2.0 + 3.0 + 5.0	10	±1.0	3, 5, 12, 13, 15, 18
Methylene blue	analogous EPA 425.1, APHA 5540 C, ASTM 2330-02, DIN EN 903, ISO 7875-1	5.0	–	±0.09	9, 11, 13, 18
Disulfine blue	analogous DIN 38409-20	0.5 + 5.0	–	±0.06	9, 11, 13, 18
TBPE	–	4.0	–	±0.26	9, 11, 13, 18
–	physical measurement	–	20	–	

Areas of application:	3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
	4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	5 Boiler water, cooling water	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	6 Construction-material industry	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater

Spectroquant® Test Kits

Parameters T-Z

	Parameter	Measuring range of the Spectroquant® instruments [mg/L]				Citation form	No. of tests	Ord. No.
		Prove 100/300/600	NOVA 30/60	Multy	Move 100			
T	Tin Cell Test	0.10 – 2.50	0.10 – 2.50 •	0.10 – 2.50	0.10 – 2.50	Sn	25	1.14622.0001
	TOC Cell Test	5.0 – 80.0	5.0 – 80.0	5.0 – 80.0	–	TOC	25	1.14878.0001
	TOC Cell Test	50 – 800	50 – 800	50 – 800	–	TOC	25	1.14879.0001
	Screw caps for Spectroquant® TOC digestion	–	–	–	–	–	6	1.73500.0001
	TOC-Standard 1000 ±10 mg/L	–	–	–	–	–	100 mL	1.09017.0100
	Total Alkalinity							
	Total Hardness Cell Test	5 – 215	5 – 215	5 – 215	5 – 215	Ca	25	1.00961.0001
		0.7 – 30.1	0.7 – 30.1	0.7 – 30.1	0.7 – 30.1	°d		
		0.9 – 37.6	0.9 – 37.6	0.9 – 37.6	0.9 – 37.6	°e		
		1.2 – 53.7	1.2 – 53.7	1.2 – 53.7	1.2 – 53.7	°f		
		7 – 301	7 – 301	7 – 301	7 – 301	CaO		
		12 – 537	12 – 537	12 – 537	12 – 537	CaCO ₃		
	Total Nitrogen							
	Transmission	0.0 – 100.0 %	0.0 – 100.0 %	–	–	T	–	–
	Turbidity	1 – 100	1 – 100 •	1 – 100	1 – 100	FAU	–	–
V	Volatile Organic Acid Cell Test	50 – 3,000	50 – 3,000	50 – 3,000	50 – 3,000	acetic acid	25	1.01749.0001
		71 – 4,401	71 – 4,401	71 – 4,401	71 – 4,401	butyric acid		
	Volatile Organic Acid Test ^{A)}	50 – 3,000	50 – 3,000	50 – 3,000	50 – 3,000	acetic acid	100	1.01809.0001
		71 – 4,401	71 – 4,401	71 – 4,401	71 – 4,401	butyric acid		
W	Water Hardness							
Z	Zinc Cell Test ^{C)}	0.025 – 1.000	0.025 – 1.000	25 – 1,000 µ/L	25 – 1,000 µ/L	Zn	25	1.00861.0001
	Zinc Test ^{C)}	0.05 – 2.50	0.05 – 2.50 •	–	–	Zn	100	1.14832.0001
	Zinc Reagent 6 (Isobutylmethylketone GR)	–	–	–	–	–	200	1.06146.1000
	Zinc Cell Test ^{C)}	0.20 – 5.00	0.20 – 5.00	0.20 – 5.00	0.20 – 5.00	Zn	25	1.14566.0001



Visit our E-shop

All our products for water, food and environmental analytics are available online – day or night. For further details and easy shopping, please visit

www.sigma-aldrich.com

^{A.} The cell test contains four 16 mm cells with a bar-code label. After measurement, the cells can be emptied and cleaned for subsequent measurements. | ^{C.} For determination of total content of this parameter, use one of the Crack Sets before the photometric procedure, see page 51. | • Only with NOVA 60



TOC TEST

Easily check total organic carbon
with our TOC cell test

www.merckmillipore.com/photometry

Method	Reference to norms and standards / Comments	Pipette volume [mL]	Cell size [mm] NOVA/Prove	Accuracy [mg/L]	Areas of application
Pyrocatechol violet	–	5.0	–	±0.08	5, 10, 16, 18
Indicator	Oxidation analogous APHA 5310 D	3.0 + 25	–	±3.6	9, 11, 13, 15, 18
Indicator	Oxidation analogous APHA 5310 D	1.0 + 3.0 + 9.0	–	±40	8, 11, 13, 18
–	for multiple use, additionally required for TOC measurement	–	–	–	
–	analogous EN 1484-H43, DIN 38409-H3 see Acid Capacity to pH 4.3	–	–	–	
Phthalein complexone	–	1.0	–	±8	2, 9, 13, 15
	see Nitrogen (total)				
–	–	10, 20, 50	–	–	
–	analogous to EN ISO 7027	–	50	–	
Hydroxamic acids / iron(III) salt	–	0.5 + 5.0	–	±69	4, 8, 11, 18
Hydroxamic acids / iron(III) salt	–	0.75 + 0.5 + 5.0	–	±85	4, 8, 11, 18
	see Total Hardness or Res. Hardness				
PAR	–	0.5 + 2.0 + 10	–	±0.033	1, 5, 9, 10, 11, 13, 15, 18
Cl-PAN	–	5.0	10	±0.07	5, 6, 8, 9, 10, 11, 15, 18
–	Extracting agent for Zinc Test 1.14832.0001	–	–	–	
PAR	–	0.5	–	±0.18	5, 6, 8, 9, 10, 11, 15, 18

Areas of application:


3	Beverages	7	Disinfection control	11	Environment	15	Mineral water
4	Biotechnology, fermenter	8	Disposal drainage water	12	Food testing	16	Seawater
1	Agriculture	9	Drinking water	13	Groundwater, surface water	17	Swimming pools
2	Aquaculture	10	Electroplating surface refinement	14	Milk dairy products	18	Wastewater
5	Boiler water, cooling water						
6	Construction-material industry						

Spectroquant® Test Kits for other photometer brands

We also offer **Spectroquant® test kits** that work seamlessly with other photometer brands. The tests don't need device-specific calibration as they use the original programs installed by the manufacturers, and work according to the instrument's operation manual. This means you can still benefit from our quality documentation when using other photometer brands. Simply download the batch certificate from: www.merckmillipore.com/coa.

Test kits for other photometer brands | Overview A-Z

Parameter	Measuring range [mg/L]	No. of tests	Merck Ord. No.	Hach Ord. No.
C Chlorine Powder Packs for photometers of other manufacturers for 10-mL-samples (free Chlorine)	0 – 2.00 Cl ₂	100	1.19254.0001	21055-69 21055-28
Chlorine Powder Packs for photometers of other manufacturers for 25-mL-samples (free Chlorine)	0 – 10.00 Cl ₂	100	1.19256.0001	14070-99 14070-28
Chlorine Powder Packs for photometers of other manufacturers for 10-mL-samples (total Chlorine)	0 – 2.00 Cl ₂	100	1.19257.0001	21056-69 21056-28
Chlorine Powder Packs for photometers of other manufacturers for 25-mL-samples (total Chlorine)	0 – 10.00 Cl ₂	100	1.19258.0001	14064-99 14064-28
USEPA approved COD Cell Tests for photometers of other manufacturers	0 – 40.0 COD	25	1.18750.0001	24158-25 24158-15 24158-51
USEPA approved COD Cell Tests for photometers of other manufacturers	0 – 150.0 COD	25	1.18751.0001	21258-25 21258-15 21258-51
USEPA approved COD Cell Tests for photometers of other manufacturers	0 – 1,500 COD	25	1.18752.0001	21259-25 21259-15 21259-51
USEPA approved COD Cell Tests for photometers of other manufacturers	0 – 15,000 COD	25	1.18753.0001	24159-25 24159-15 24159-51
O Oxygen Scavengers Test	0.020 – 0.500 DEHA 0.027 – 0.667 Carbohy 0.053 – 1.315 Hydro 0.078 – 1.950 ISA 0.087 – 2.170 MEKO	200	1.19251.0001	24466-00
S Sulfate Powder Packs for photometers of other manufacturers for 25-mL-samples	0 – 70.0 SO ₄	100	1.73015.0001	12065-99 12065-28

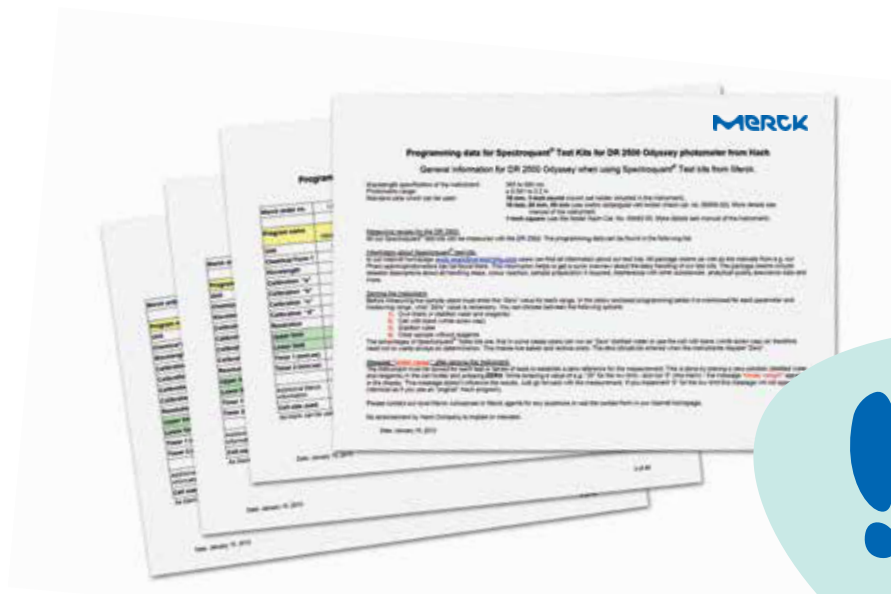

By the way ...

All Spectroquant® test kits can be programmed to work with any manufacturer's photometer. Simply download the programming data from: www.service-test-kits.com

Method	Reference to norms and standards / Comments	Pipette-volume	Cell size Hach	Areas of application
DPD	analogous EPA 330.5, APHA 4500-Cl G	10 mL	1 inch	2, 7, 9, 11, 13, 16, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl G	25 mL	1 inch	2, 7, 9, 11, 13, 16, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl G	10 mL	1 inch	2, 7, 9, 11, 13, 16, 17, 18
DPD	analogous EPA 330.5, APHA 4500-Cl G	25 mL	1 inch	2, 7, 9, 11, 13, 16, 17, 18
Oxidation with Chromosulfuric acid, determination as chromate	analogous EPA 410.4, APHA 5220 D, ISO 15705 and ASTM D1252-06B	2.0 mL	16 mm	5, 9, 10, 11, 13, 15, 17, 18
Oxidation with Chromosulfuric acid, determination as chromate	analogous EPA 410.4, APHA 5220 D, ISO 15705 and ASTM D1252-06B	2.0 mL	16 mm	5, 9, 10, 11, 13, 15, 17, 18
Oxidation with Chromosulfuric acid, determination as chromate	analogous EPA 410.4, APHA 5220 D, ISO 15705 and ASTM D1252-06B	2.0 mL	16 mm	3, 4, 5, 8, 10, 11, 13, 18
Oxidation with Chromosulfuric acid, determination as chromate	analogous EPA 410.4, APHA 5220 D, ISO 15705 and ASTM D1252-06B	0.2 mL	16 mm	3, 4, 5, 8, 10, 11, 13, 18
Iron Reduction		2.0 mL + 10 mL	1 inch	5
Barium chloride	analogous EPA 375.4	25 mL	1 inch	1, 5, 6, 7, 8, 9, 10, 11, 13, 15, 18

Areas of application:

3 Beverages	7 Disinfection control	11 Environment	15 Mineral water
4 Biotechnology, fermenter	8 Disposal drainage water	12 Food testing	16 Seawater
1 Agriculture	9 Drinking water	13 Groundwater, surface water	17 Swimming pools
2 Aquaculture	10 Electroplating surface refinement	14 Milk dairy products	18 Wastewater
5 Boiler water, cooling water			
6 Construction-material industry			

Spectroquant® Test Kits for samples with high salt content

Higher salt content may interfere with the reagents of test kits developed for drinking water and wastewater. The following tables help you choose the most **suitable Spectroquant® test kits for analyzing seawater and samples with high salt content**. Select the test kit with your required parameter to learn about its tolerance limits for neutral salts, and its suitability for analyzing seawater.

Over 250
applications

on www.merckmillipore.com/aaf
> **Photometry**

M ANY
SOLUTIONS
for all application fields

EASY, FAST
AND RELIABLE
methods for your convenience

Be unlimited



COD test for seawater/high chloride content

- First COD test with unlimited chloride tolerance
- No need to titrate or dilute samples
- Suitable for testing seawater, and municipal or industrial wastewater
- Lower range: 5 – 60 mg/L COD
[Ord. No. 1.17058.0001]
- Higher range: 50 – 3,000 mg/L COD
[Ord. No. 1.17059.0001]
- Easy, fast and precise

More details on pages 64 and 84

Suitability of test kits for testing seawater and tolerance limits for neutral salts | Overview A-C

Test kit		Ord. No.	Seawater	Tolerance limit, salts in %		
				NaCl	NaNO ₃	Na ₂ SO ₄
A	Acid Capacity Cell Test	1.01758.0001	no	–	–	–
	Aluminium Cell Test	1.00594.0001	yes	20	20	20
	Aluminium Test	1.14825.0001	yes	10	20	20
	Ammonium Cell Test	1.14739.0001	no	5	5	5
	Ammonium Cell Test	1.14558.0001	yes	20	10	15
	Ammonium Cell Test	1.14544.0001	yes	20	15	20
	Ammonium Cell Test	1.14559.0001	yes	20	20	20
	Ammonium Test	1.14752.0001	no ¹⁾	10	10	20
		1.14752.0002				
	Ammonium Test	1.00683.0001	yes	20	20	20
	AOX Cell Test	1.00675.0001	no	0.4	20	20
	Arsenic Test	1.01747.0001	no	10	10	10
B	BOD Cell Test	1.00687.0001	yes	20	20	20
	Boron Cell Test	1.00826.0001	yes	10	20	20
	Boron Test	1.14839.0001	no	20	5	20
	Bromine Test	1.00605.0001	no	10	10	10
C	Cadmium Cell Test	1.14834.0001	no	1	10	1
	Cadmium Test	1.01745.0001	no	1	10	1
	Calcium Cell Test	1.00858.0001	no	2	2	1
	Calcium Test	1.14815.0001	yes	20	20	10
	Calcium Test	1.00049.0001	no	–	–	–
	Chloride Test	1.01807.0001	no	–	0.5	0.05
	Chloride Cell Test	1.01804.0001	no	–	0.5	0.05
	Chloride Cell Test	1.14730.0001	yes	–	20	1
	Chloride Test	1.14897.0001	yes	–	10	0.1
		1.14897.0002				
	Chlorine Cell Test	1.00595.0001	no	10	10	10
	Chlorine Cell Test	1.00597.0001	no	10	10	10
	Chlorine Test	1.00598.0001	no	10	10	10
		1.00598.0002				
	Chlorine Test	1.00602.0001	no	10	10	10
		1.00602.0002				
	Chlorine Test	1.00599.0001	no	10	10	10
	Chlorine Reagent (liquid) (free and total)	1.00086.0001	no	10	10	10
		1.00087.0001				
		1.00088.0001				
	Chlorine dioxide Test	1.00608.0001	no	10	10	10
	Chromate Cell Test (Chromium VI)	1.14552.0001	yes	10	10	10
	Chromium (total) Cell Test	1.14552.0001	no	1	10	10
	Chromate Test	1.14758.0001	yes	10	10	10

¹⁾ This test kit is also suitable for testing seawater after the addition of sodium hydroxide solution (see package insert).

Spectroquant® Test Kits for samples with high salt content

Suitability of test kits for testing seawater and tolerance limits
for neutral salts | Overview C-L

	Test kit	Ord. No.	Seawater	Tolerance limit, salts in %		
				NaCl	NaNO ₃	Na ₂ SO ₄
C	COD Cell Test	1.14560.0001	no	0.4	10	10
	COD Cell Test	1.01796.0001	no	0.4	10	10
	COD Cell Test	1.14540.0001	no	0.4	10	10
	COD Cell Test	1.14895.0001	no	0.4	10	10
	COD Cell Test	1.14690.0001	no	0.4	20	20
	COD Cell Test	1.14541.0001	no	0.4	10	10
	COD Cell Test	1.14691.0001	no	0.4	20	20
	COD Cell Test	1.14555.0001	no	1.0	10	10
	COD Cell Test	1.01797.0001	no	10	20	20
	COD Cell Test for seawater / high chloride contents	1.17058.0001	yes	35	10	10
	COD Cell Test for seawater / high chloride contents	1.17059.0001	yes	35	10	10
	COD Cell Test (Hg free)	1.09772.0001	no	0	10	10
	COD Cell Test (Hg free)	1.09773.0001	no	0	10	10
	Copper Cell Test	1.14553.0001	yes	15	15	15
	Copper Test	1.14767.0001	yes	15	15	15
	Cyanide Cell Test	1.02531.0001	no	10	10	10
	Cyanide Cell Test	1.14561.0001	no	10	10	10
	Cyanide Test	1.09701.0001	no	10	10	10
	Cyanuric Acid Test	1.19253.0001	yes	–	–	–
F	Fluoride Test	1.00822.0250	yes ²⁾	0.05	0.05	0.001
	Fluoride Cell Test	1.00809.0001	no	10	10	10
	Fluoride Test	1.14598.0001	yes	20	20	20
		1.14598.0002				
	Formaldehyde Cell Test	1.14500.0001	no	5	0	10
	Formaldehyde Test	1.14678.0001	no	5	0	10
G	Gold Test	1.14821.0002	yes	10	20	5
H	Hardness, see Total Hardness Cell Test					
	Hydrazine Test	1.09711.0001	no	20	5	2
	Hydrogen Peroxide Cell Test	1.14731.0001	yes	20	20	20
	Hydrogen Peroxide Test	1.18789.0001	no	0.1	1	5
	Iodine Test	1.00606.0001	no	10	10	10
	Iron Cell Test	1.14549.0001	yes	20	20	20
I	Iron Cell Test	1.14896.0001	no	5	5	5
	Iron Test	1.14761.0001	yes	20	20	20
		1.14761.0002				
	Iron Test	1.00796.0001	yes	20	20	20
	Lead Cell Test	1.14833.0001	no	20	20	1
L	Lead Test	1.09717.0001	no	20	5	15

²⁾ Distill beforehand as per APHA 4400-F B



ANALYTICAL APPLICATION NOTES FINDER

Interested in more application examples?
Visit: www.merckmillipore.com/aaf > Photometry

www.merckmillipore.com/photometry

Suitability of test kits for testing seawater and tolerance limits for neutral salts | Overview M-P

	Test kit	Ord. No.	Seawater	Tolerance limit, salts in %		
				NaCl	NaNO ₃	Na ₂ SO ₄
M	Magnesium Cell Test	1.00815.0001	yes	2	2	1
	Manganese Test	1.00816.0001	no	20	20	20
	Manganese Test	1.01846.0001	no	20	25	5
	Manganese Test	1.14770.0001	yes	20	20	20
		1.14770.0002				
	Molybdenum Cell Test	1.00860.0001	no	20	20	5
N	Monochloramine Test	1.01632.0001	no	10	10	20
	Nickel Cell Test	1.14554.0001	no	20	20	20
	Nickel Test	1.14785.0001	no	20	20	20
	Nitrate Cell Test	1.14542.0001	no	0.4	–	20
	Nitrate Cell Test	1.14563.0001	no	0.2	–	20
	Nitrate Cell Test	1.14764.0001	no	0.5	–	20
	Nitrate Cell Test	1.00614.0001	no	2	–	20
	Nitrate Test	1.01842.0001	no	0.001	–	0.001
	Nitrate Test	1.14773.0001	no	0.4	–	20
	Nitrate Test	1.09713.0001	no	0.2	–	20
		1.09713.0002				
	Nitrate Cell Test (seawater)	1.14556.0001	yes	20	–	20
	Nitrate Test (seawater)	1.14942.0001	yes	20	–	20
	Nitrite Cell Test	1.14547.0001	yes	20	20	15
	Nitrite Cell Test	1.00609.0001	yes	20	20	15
	Nitrite Test	1.14776.0001	yes	20	20	15
		1.14776.0002				
	Nitrogen (total) Cell Test	1.14537.0001	no	0.5	–	10
	Nitrogen (total) Cell Test	1.00613.0001	no	0.2	–	10
	Nitrogen (total) Cell Test	1.14763.0001	no	2	–	20
O	Oxygen Cell Test	1.14694.0001	no	10	5	1
	Oxygen Scavengers Test	1.19251.0001	no	–	–	–
	Ozone Test	1.00607.0001	no	10	10	10
P		1.00607.0002				
	pH Cell Test	1.01744.0001	yes	–	–	–
	Phenol Cell Test	1.14551.0001	yes	20	20	15
	Phenol Test	1.00856.0001	yes	20	20	20
	Phosphate (ortho-phosphate) Cell Test	1.00475.0001	yes	20	20	20
	Phosphate (ortho-phosphate) Cell Test	1.14543.0001	yes	5	10	10
	Phosphorus (total) Cell Test	1.14543.0001	no	1	10	10
	Phosphate (ortho-phosphate) Cell Test	1.00474.0001	yes	5	10	10
	Phosphate (ortho-phosphate) Cell Test	1.14729.0001	yes	20	20	20
	Phosphorus (total) Cell Test	1.14729.0001	yes	5	20	20

Spectroquant® Test Kits for samples with high salt content

Suitability of test kits for testing seawater and tolerance limits
for neutral salts | Overview P-Z

	Test kit	Ord. No.	Seawater	Tolerance limit, salts in %		
				NaCl	NaNO ₃	Na ₂ SO ₄
P	Phosphate (ortho-phosphate) Cell Test	1.00616.0001	yes	20	20	20
	Phosphate (ortho-phosphate) Cell Test	1.00673.0001	yes	20	20	20
	Phosphorus (total) Cell Test	1.00673.0001	yes	20	20	20
	Phosphate Test	1.14848.0001	yes	5	10	10
		1.14848.0002				
	Phosphate Test	1.00798.0001	yes	15	20	10
	Phosphate Cell Test	1.14546.0001	yes	20	20	20
	Phosphate Test	1.14842.0001	yes	20	20	20
	Potassium Cell Test	1.14562.0001	yes	20	20	20
R S	Potassium Cell Test	1.00615.0001	yes	20	20	20
	Residual Hardness Cell Test	1.14683.0001	no	0.01	0.01	0.01
	Silicate (Silicic Acid) Test	1.01813.0001	no	0.5	1	0.2
	Silicate (Silicic Acid) Test	1.14794.0001	yes	5	10	5
	Silicate (Silicic Acid) Test	1.00857.0001	no	5	10	2.5
	Silver Test	1.14831.0001	no	0	1	5
	Sodium Cell Test	1.00885.0001	no	–	10	1
	Sulfate Test	1.01812.0001	no	2	0.007	–
	Sulfate Cell Test	1.14548.0001	yes	10	0.1	–
	Sulfate Cell Test	1.00617.0001	yes	10	0.1	–
	Sulfate Cell Test	1.14564.0001	yes	10	0.5	–
	Sulfate Cell Test	1.02537.0001	yes	10	0.015	–
		1.02537.0002				
	Sulfate Test	1.02532.0001	no	2	0.007	–
	Sulfate Test	1.14791.0001	no	0.2	0.2	–
	Sulfide Test	1.14779.0001	no	0.5	1	1
	Sulfite Cell Test	1.14394.0001	no	20	20	20
	Sulfite Test	1.01746.0001	no	20	20	20
	Surfactants (anionic) Cell Test	1.02552.0001	no	0.1	0.01	10
	Surfactants (cationic) Cell Test	1.01764.0001	no	0.1	0.1	20
	Surfactants (nonionic) Cell Test	1.01787.0001	no	2	5	2
T	Tin Cell Test	1.14622.0001	yes	20	20	20
	TOC Cell Test	1.14878.0001	no	0.5	10	10
	TOC Cell Test	1.14879.0001	no	5	20	20
	Total Hardness Cell Test	1.00961.0001	no	2	2	1
V	Volatile Organic Acid Cell Test	1.01749.0001	no	20	20	10
	Volatile Organic Acid Test	1.01809.0001	no	20	20	10
Z	Zinc Cell Test	1.00861.0001	no	20	20	1
	Zinc Cell Test	1.14566.0001	no	10	10	10
	Zinc Test	1.14832.0001	no	5	15	15

Be flexible



Broad measuring range for flexible sulfate testing

- Sulfate is essential for human health
- But high sulfate levels in tap water can cause pipe corrosion or bursting, and diminish water quality
- Maximum limit set by regulatory agencies: approx. 250 mg/L
- Spectroquant® sulfate test with range of 5–300 mg/L is ideal for testing low sulfate in bottled water or high content in tap water
- Cost-efficient test with 100 or 1000 determinations per pack
- Alternatively, Spectroquant® cell test contains 25 prefilled cells for greater convenience

• **Spectroquant® Sulfate Test** [Ord. No. 1.02537.0001]

• **Spectroquant® Sulfate Cell Test** [Ord. No. 1.02532.0001]

More applications for your convenience can be downloaded from our Application Notes Finder: www.merckmillipore.com/aaf

Be sure

Sensitive, secure measurement of phosphate

- Phosphate is essential for plants and animals
- But phosphate content in ground and surface water should be as low as possible to avoid eutrophication (excess algal growth) and environmental risks
- With Spectroquant® Prove 600 and 100-mm cells, levels as low as 2.5 µg/L PO₄-P can be measured, corresponding to DIN EN ISO 6878, 4500 P and EPA 365.2+3
- Spectroquant® Phosphate Test [Ord. No. 1.14848.0001]

Learn more on page 74 and 85




Spectroquant® Analytical Quality Assurance

SIMPLY COMPLETE

Analytical Quality Assurance [AQA] is the practice of ensuring that your results are reliable and conform with Good Laboratory Practice (GLP) guidelines. This thorough process includes installation qualification (IQ), operational qualification (OQ), and performance qualification (PQ).

The Spectroquant® AQA concept covers all stages of internal quality control (IQC). We also provide complete IQ, OQ and PQ documentation for all Spectroquant® instruments. Target values and tolerances are either supplied in certificates or pre-programmed in the instruments.

Installation Qualification [IQ] aims to verify that instrument delivery matches the purchase order, and to assure that it is installed correctly.

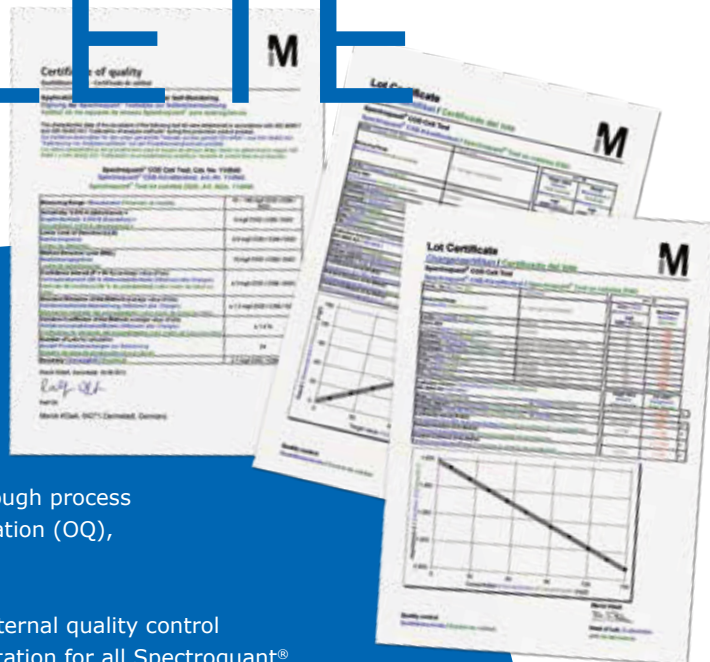

AQA 3 steps to great quality

1

PHOTOMETER CHECK: Operational qualification (OQ)
Easy to perform with certified color standards, or Certipur® UV/Vis standards

2

SYSTEM CHECK: Performance qualification (PQ)
Recovery measurement using CombiCheck standard solution, certified reference material (CRM) standard solutions, or Certipur® standard solutions

3

MATRIX CHECK: Performance qualification (PQ)
One-time spiking with CombiCheck R-2 solution, or multiple dilution/spiking with certified reference material (CRM) standard solutions or self-prepared solutions.

PHOTOMETER CHECK

AQA 1

Operational qualification (OQ) – Checking the instrument

The aim of OQ is to assure the instrument's functionality over the entire operating range, according to defined procedures.

Photometer Check

All Spectroquant® instruments are checked using certified color standards, or Certipur® UV/Vis standards.

Spectroquant® NOVA and Spectroquant® Prove photometers

These photometers offer an instrument-supported AQA concept that combines the three essential components of quality control. For effortless, accurate AQA – **target values and tolerances are on the certificate, and can be stored and used for further checks.**



100 | 300 | 600
30 | 60 | 60A
100
Cl₂/O₃/ClO₂/CYA/pH

Photometer Check	Information	Content	Ord. No.	Prove	NOVA	Move	Multy
Spectroquant® Zero Cell	We recommend replacing the zero cell every 2 years.	One 16-mm cell filled with distilled water	1.73503.0001	■	■		
Spectroquant® PhotoCheck	Secondary standards are compliant with ISO 9001, ISO 14001 and ISO 17205 guidelines, and calibrated with instrument qualified with NIST standards.	- Check solutions for 3 different wavelengths 2 zero cells 2 cells for checking the bar-code reader (only for Spectroquant® NOVA photometers)	1.14693.0001	■	■		
Spectroquant® Verification Standards	Standards are supplied in sealed vials, which are individually calibrated on instruments traceable to NIST SRM 2032, 935a.	1 zero standard 6 cells for checking 6 different wavelengths of the instrument	1.19302.0001			■	■
Spectroquant® Reference Standards	Standards are supplied in sealed vials, which are individually calibrated on instruments traceable to NIST SRM 2032, 935a.	1 zero standard 3 cells for checking 3 different concentrations for chlorine, chlorine dioxide and ozone method in the instrument	1.19301.0001			■	
Spectroquant® PipeCheck	For checking pipettes and documenting results, without the need for a precise balance.	24 cells with check solutions 4 cells with corresponding reference solutions	1.14962.0001	■	■	■	■

Spectroquant® Analytical Quality Assurance

Certipur® UV/Vis standards

Certipur® UV/Vis standards can be used to verify the consistent and correct operation of your UV/Vis spectrophotometer. The solutions are suitable for checking the following parameters as per Ph Eur:

- Absorption
- Stray light
- Wavelength accuracy

Operations as per GLP, GMP, USP and ISO 9001 or ISO 45001 demand these regular controls.

All standards are traceable to NIST.



Designation	Content	Ord. No.	Prove 100	Prove 300	Prove 600
UV/Vis Standard 1	Potassium dichromate solution for absorbance acc. to DAB and Ph Eur Certipur® 2 x 10 mL K ₂ Cr ₂ O ₇ – 60.06 mg/L in H ₂ SO ₄ – 0.01 N and 6 x 10 mL H ₂ SO ₄ – 0.01 N	1.08160.0001	■	■	■
UV/Vis Standard 1A	Potassium dichromate solution for absorbance at 430 nm acc. to DAB and Ph Eur Certipur® 2 x 10 mL K ₂ Cr ₂ O ₇ – 600.06 mg/L in H ₂ SO ₄ – 0.01 N and 6 x 10 mL H ₂ SO ₄ – 0.01 N	1.04660.0001	■	■	■
UV/Vis Standard 2	Sodium nitrite solution for stray light testing acc. to DAB and Ph Eur Certipur® 3 x 10 mL NaNO ₂ – 50 g/L in H ₂ O	1.08161.0001	■	■	■
UV/Vis Standard 3	Sodium iodide solution for stray light testing acc. to DAB and Ph Eur Certipur® 3 x 10 mL NaI – 10 g/L in H ₂ O	1.08163.0001			■
UV/Vis Standard 4	Potassium chloride solution for stray light testing acc. to DAB and Ph Eur Certipur® 3 x 10 mL KCl – 12 g/L in H ₂ O	1.08164.0001			■
UV/Vis Standard 5	Toluene solution in n-hexane for testing the resolution power acc. to DAB and Ph Eur Certipur® 2 x 10 mL 0.02 % (v/v) toluene and 6 x 10 mL n-hexane	1.08165.0001			■
UV/Vis Standard 6	Holmium oxide solution reference material for wavelength testing acc. to DAB and Ph Eur Certipur® 3 x 10 mL Ho ₂ O ₃ – 40 g/L in HClO ₄ (10 % v/v)	1.08166.0001	■	■	■

SYSTEM CHECK

AQA 2

Performance qualification [PQ] – Checking the complete system and sample matrix

Verifying product-related functionalities is the most comprehensive step in the process, and involves the measurement of both method-specific standards and real samples. PQ consists of two components: System Check and Matrix Check.

System Check

System Check covers all components of the analysis (instrument, test kit, standard, pipette and/or cell, and operator).

► The recommended standard solutions for each Spectroquant® test kit are listed on page 92 – 97.

► Spectroquant® CombiCheck Product information see page 98 – 101

► Standard solutions (CRM) for photometric applications Product information see page 102

► Certipur® standard solution Product information see page 106

MATRIX CHECK

AQA 3

What: Matrix Check, identifies measurement errors due to interferences from foreign substances in the sample. As they can significantly interfere with results, various foreign substances have been investigated to define the maximum concentration at which they may be present in samples without causing errors. These limits are stated in the package insert of each Spectroquant® test kit.

Why: For samples with very complex or unknown compositions, interferences can be analyzed based on recovery rates, and rectified through appropriate countermeasures, such as sample pre-treatment.

How: Depending on the sample concentration, there are two methods to choose from:

1. One-time standard addition (spiking) with CombiCheck R-2 addition solution

► Spectroquant® CombiCheck

Product information see page 98 – 101

2. Multiple dilutions or spiking with self-prepared spiking solutions

To avoid changing the sample matrix, spiking solutions should be highly concentrated standards, and used in small quantities relative to the sample portion.

► Standard solutions (CRM) for photometric applications

Product information see page 102

► Certipur® standard solution

Product information see page 106

Comprehensive quality assurance using IQ, OQ, and PQ documents will transform your measurements into proven, verifiable analytical results. **Please contact your local Merck representative to learn more about our quality assurance service.**

PROTECT YOUR DATA

Password-protected control of the complete system

- Ensure AQA intervals are observed by issuing a password (NOVA photometers), or defining hierarchical user groups (Prove spectrophotometers)
- Measurements and methods are only possible if quality control checks and intervals are adhered to
- Documentation of AQA results are provided in the final report, proving GLP compliance and ensuring that the system is tested



Spectroquant® Analytical Quality Assurance

The following tables show you the most suitable test kits for different quality assurance parameters. In cases where a parameter is not stable (e.g. chlorine), we provide application instructions for preparing the standard. These can be found in the preface of our photometer and colorimeter manuals, or on www.merckmillipore.com/photometry. Comprehensive overview of standard solutions you can find from our e-shop www.sigma-aldrich.com and page 104.

Parameters A-B

Test kit	Ord. No. Test kit	Ord. No. CombiCheck	Ord. No. Standard solution, CRM	Alternative Standard	Ord. No. Certipur® standard sol.
A Acid Capacity Cell Test to pH 4.3 (total alkalinity)	1.01758.0001			²⁾	
Aluminium Cell Test	1.00594.0001	1.18701.0001	1.32226.0100	¹⁾	1.19770.0100
Aluminium Test	1.14825.0001	1.18701.0001	1.32225.0100	¹⁾	1.19770.0100
Ammonium Cell Test	1.14739.0001	1.14695.0001	1.25022.0100 1.25023.0100	¹⁾	1.19812.0500
Ammonium Cell Test	1.14558.0001	1.14676.0001	1.25022.0100 1.25023.0100 1.25024.0100 1.25025.0100	¹⁾	1.19812.0500
Ammonium Cell Test	1.14544.0001	1.14675.0001	1.25023.0100 1.25024.0100 1.25025.0100 1.25026.0100	¹⁾	1.19812.0500
Ammonium Cell Test	1.14559.0001	1.14689.0001	1.25025.0100 1.25026.0100 1.25027.0100	¹⁾	1.19812.0500
Ammonium Test	1.14752.0001 1.14752.0002	1.14695.0001	1.25022.0100 1.25023.0100 1.25024.0100	¹⁾	1.19812.0500
Ammonium Test	1.00683.0001	1.14689.0001	1.25025.0100 1.25026.0100 1.25027.0100	¹⁾	1.19812.0500
AOX Cell Test	1.00675.0001			0.2 – 2.0 mg/L AOX 1.00680.0001	
Arsenic Test	1.01747.0001		1.33002.0250	¹⁾	1.19773.0100
B BOD Cell Test	1.00687.0001			EN 1899, 210 mg/L 1.00718.0001	
Boron Cell Test	1.00826.0001		1.33005.0100	¹⁾	1.19500.0100
Boron Test	1.14839.0001			¹⁾	1.19500.0100
Bromate			1.33006.0100 1.33007.0100	²⁾	
Bromine Test	1.00605.0001			DIN EN ISO 7393 ²⁾	

¹⁾ Standard solution, ready-to-use, 1,000 mg/L analyt. Traceable to SRM of NIST (see Ord. No. Certipur® standard solution) | ²⁾ Own standards. Worksheets how to prepare these standards can be downloaded from our website www.merckmillipore.com/aaf > Photometry > Field of Activity/Sample = Standard | ³⁾ For photometers of other manufacturers

Parameters C

Test kit	Ord. No. Test kit	Ord. No. CombiCheck	Ord. No. Standard solution, CRM	Alternative Standard	Ord. No. Certipur® standard sol.
C Cadmium Cell Test	1.14834.0001	1.18700.0001	1.32228.0100	¹⁾	1.19777.0100
Cadmium Test	1.01745.0001	1.18700.0001	1.32228.0100		1.19777.0100
Calcium Cell Test	1.00858.0001			NIST3109A ²⁾	
Calcium Test	1.00049.0001			¹⁾	1.19778.0100
Calcium Test	1.14815.0001			¹⁾	1.19778.0100
Chloride Cell Test	1.01804.0001		1.33010.0100	¹⁾	1.19897.0500
Chloride Cell Test	1.14730.0001	1.14676.0001 1.14675.0001	1.32229.0100 1.32230.0100	¹⁾	1.19897.0500
Chloride Test	1.01807.0001		1.33010.0100	¹⁾	1.19897.0500
Chloride Test	1.14897.0001 1.14897.0002	1.14696.0001	1.32229.0100 1.32230.0100	¹⁾	1.19897.0500
Chlorine Cell test (free)	1.00595.0001			DIN EN ISO 7393 ²⁾	
Chlorine Test (free)	1.00598.0002 1.00598.0001			DIN EN ISO 7393 ²⁾	
Chlorine Test (total)	1.00602.0001 1.00602.0002			DIN EN ISO 7393 ²⁾	
Chlorine Cell Test (free and total)	1.00597.0001			DIN EN ISO 7393 ²⁾	
Chlorine Test (free and total)	1.00599.0001			DIN EN ISO 7393 ²⁾	
Chlorine Powder Packs ³⁾ (free)	1.19254.0001 1.19256.0001			DIN EN ISO 7393 ²⁾	
Chlorine Powder Packs ³⁾ (total)	1.19257.0001 1.19258.0001			DIN EN ISO 7393 ²⁾	
Chlorine Dioxide Test	1.00608.0001			DIN EN ISO 7393 ²⁾	
Chromate Cell Test	1.14552.0001		1.33013.0100	¹⁾	1.19780.0500
Chromate Test	1.14758.0001		1.33012.0100	¹⁾	1.19780.0500
COD Cell Test	1.14560.0001	1.14695.0001	1.25028.0100	²⁾	
COD Cell Test	1.01796.0001	1.14695.0001	1.25028.0100	²⁾	
COD Cell Test	1.14540.0001	1.14676.0001	1.25029.0100	²⁾	
COD Cell Test	1.14895.0001	1.14696.0001	1.25029.0100 1.25030.0100	²⁾	
COD Cell Test	1.14690.0001	1.14696.0001	1.25029.0100 1.25030.0100 1.25031.0100	²⁾	
COD Cell Test	1.14541.0001	1.14675.0001	1.25029.0100 1.25030.0100 1.25031.0100 1.25032.0100	²⁾	
COD Cell Test	1.14691.0001	1.14738.0001	1.25031.0100 1.25032.0100 1.25033.0100	²⁾	
COD Cell Test	1.14555.0001	1.14689.0001	1.25032.0100 1.25033.0100 1.25034.0100	²⁾	
COD Cell Test	1.01797.0001		1.25035.0100	²⁾	

Spectroquant® Analytical Quality Assurance

Parameters C-M

Test kit	Ord. No. Test kit	Ord. No. CombiCheck	Ord. No. Standard solution, CRM	Alternative Standard	Ord. No. Certipur® standard sol.
C COD Cell Test (Hg-free)	1.09772.0001		1.25028.0100 1.25029.0100	²⁾	
COD Cell Test (Hg-free)	1.09773.0001		1.25030.0100 1.25031.0100 1.25032.0100	²⁾	
COD Cell Test ³⁾	1.18750.0001	1.14695.0001	1.25028.0100	²⁾	
COD Cell Test ³⁾	1.18751.0001	1.14676.0001	1.25029.0100	²⁾	
COD Cell Test ³⁾	1.18752.0001	1.14675.0001	1.25029.0100	²⁾	
COD Cell Test ³⁾	1.18753.0001	1.14689.0001	1.25032.0100	²⁾	
COD Cell Test for seawater / high chloride contents	1.17058.0001			²⁾	
COD Cell Test for seawater / high chloride contents	1.17059.0001			²⁾	
Copper Cell Test	1.14553.0001	1.18700.0001		¹⁾	1.19786.0100
Copper Test	1.14767.0001	1.18700.0001			1.19786.0100
Cyanide Cell Test	1.02531.0001			¹⁾	1.19533.0500
Cyanide Cell Test	1.14561.0001			¹⁾	1.19533.0500
Cyanide Test	1.09701.0001			¹⁾	1.19533.0500
Cyanuric Acid Test	1.19253.0001			²⁾	
F Fluoride Cell Test	1.00809.0001		1.32234.0100	¹⁾	1.19814.0500
Fluoride Test	1.00822.0250		1.32234.0100	¹⁾	1.19814.0500
Fluoride Test	1.14598.0001 1.14598.0002		1.32234.0100	¹⁾	1.19814.0500
Formaldehyde Cell Test	1.14500.0001			²⁾	
Formaldehyde Test	1.14678.0001			²⁾	
G Gold Test	1.14821.0002			¹⁾	1.70216.0100
H Hydrazine Test	1.09711.0001			²⁾	
Hydrogen Peroxide Cell Test	1.14731.0001			²⁾	
Hydrogen Peroxide Test	1.18789.0001			²⁾	
I Iodine Test	1.00606.0001			DIN EN ISO 7393 ²⁾	
Iron Cell Test	1.14549.0001	1.18700.0001	1.33018.0100 1.33019.0100	¹⁾	1.19781.0100
Iron Cell Test	1.14896.0001			¹⁾	1.19781.0100
Iron Test	1.14761.0002 1.14761.0001	1.18700.0001	1.33014.0100 1.33018.0100	¹⁾	1.19781.0100
Iron Test	1.00796.0001	1.18700.0001	1.33014.0100 1.33018.0100	¹⁾	1.19781.0100
L Lead Cell Test	1.14833.0001	1.18701.0001		¹⁾	1.19776.0100
Lead Test	1.09717.0001	1.18701.0001	1.33003.0100 1.33004.0100	¹⁾	1.19776.0100
M Magnesium Cell Test	1.00815.0001		NIST 3131A	²⁾	
Manganese Cell Test	1.00816.0001	1.18700.0001	1.32238.0100	¹⁾	1.19789.0100

¹⁾ Standard solution, ready-to-use, 1,000 mg/L analyt. Traceable to SRM of NIST (see Ord. No. Certipur® standard solution) | ²⁾ Own standards. Worksheets how to prepare these standards can be downloaded from our website www.merckmillipore.com/aaf > Photometry > Field of Activity/Sample = Standard | ³⁾ For photometers of other manufacturers



ANALYTICAL APPLICATION NOTES FINDER

Interested in more application examples?

Visit: www.merckmillipore.com/aaf > Photometry

www.merckmillipore.com/photometry

Parameters M-O

Test kit	Ord. No. Test kit	Ord. No. CombiCheck	Ord. No. Standard solution, CRM	Alternative Standard	Ord. No. Certipur® standard sol.
M Manganese Test	1.01846.0001	1.18700.0001		¹⁾	1.19789.0100
	1.14770.0001	1.18700.0001	1.32237.0100	¹⁾	1.19789.0100
	1.14770.0002		1.32238.0100		
	Molybdenum Cell Test	1.00860.0001		¹⁾	1.70227.0001
Monochloramine Test	1.01632.0001			²⁾	
N Nickel Cell Test	1.14554.0001	1.18701.0001		¹⁾	1.09989.0001
	Nickel Test	1.14785.0001	1.18701.0001	¹⁾	1.09989.0001
	Nitrate Cell Test	1.14542.0001	1.14675.0001	¹⁾	1.19811.0500
			1.25037.0100		
	Nitrate Cell Test	1.14563.0001	1.14675.0001	¹⁾	1.19811.0500
			1.25037.0100		
	Nitrate Cell Test	1.14764.0001	1.14738.0001	¹⁾	1.19811.0500
			1.25037.0100		
			1.25038.0100		
	Nitrate Cell Test	1.00614.0001	1.25039.0100	¹⁾	1.19811.0500
			1.25040.0100		
	Nitrate Test	1.01842.0001	1.32241.0100	¹⁾	1.19811.0500
			1.32242.0100		
	Nitrate Test	1.14773.0001	1.14676.0001	¹⁾	1.19811.0500
			1.14675.0001		
			1.25036.0100		
	Nitrate Test	1.09713.0001	1.25037.0100	¹⁾	1.19811.0500
			1.25038.0100		
			1.25039.0100		
	Nitrate Cell Test in seawater	1.14556.0001	1.14676.0001	¹⁾	1.19811.0500
			1.25036.0100		
	Nitrate Test in seawater	1.14942.0001	1.14675.0001	¹⁾	1.19811.0500
			1.25036.0100		
			1.25037.0100		
	Nitrite Cell Test	1.14547.0001	1.25041.0100	¹⁾	1.19899.0500
			1.25042.0100		
	Nitrite Test	1.14776.0002	1.25041.0100	¹⁾	1.19899.0500
			1.33021.0100		
	Nitrite Cell Test	1.00609.0001	1.25042.0100	¹⁾	1.19899.0500
	Nitrogen (total) Cell Test	1.14537.0001	1.14695.0001	²⁾	
			1.25043.0100		
	Nitrogen (total) Cell Test	1.00613.0001	1.14695.0001	²⁾	
			1.25044.0100		
	Nitrogen (total) Cell Test	1.14763.0001	1.14689.0001	²⁾	
			1.25044.0100		
O Oxygen Cell Test	1.14694.0001			²⁾	
	Oxygen Scavengers Test	1.19251.0001		²⁾	
	Ozone-Test	1.00607.0001		DIN EN ISO 7393 ²⁾	
		1.00607.0002			

Spectroquant® Analytical Quality Assurance

Parameters P-S

Test kit	Ord. No. Test kit	Ord. No. CombiCheck	Ord. No. Standard solution, CRM	Alternative Standard	Ord. No. Certipur® standard sol.
P pH Cell Test	1.01744.0001			Buffer solution pH 7.00 / 1.09439.1000	
Phenol Cell Test	1.14551.0001			1524806 ²⁾	
Phenol Test	1.00856.0001			1524806 ²⁾	
Phosphate (ortho-phosphate) Cell Test	1.00474.0001	1.14676.0001		¹⁾	1.19898.0500
Phosphate (ortho-phosphate) Cell Test	1.14543.0001	1.14676.0001		¹⁾	1.19898.0500
Phosphorus (total) Cell Test	1.14543.0001	1.14676.0001	1.25046.0100 1.25047.0100	¹⁾	
Phosphate (ortho-phosphate) Cell Test	1.00475.0001	1.14675.0001 1.14738.0001		¹⁾	1.19898.0500
Phosphate (ortho-phosphate) Cell Test	1.14729.0001	1.14675.0001 1.14738.0001		¹⁾	1.19898.0500
Phosphorus (total) Cell Test	1.14729.0001	1.14676.0001	1.25047.0100 1.25048.0100	¹⁾	
Phosphate (ortho-phosphate) Cell Test	1.00616.0001			¹⁾	1.19898.0500
Phosphorus (total) Cell Test	1.00673.0001		1.25048.0100 1.25049.0100	¹⁾	
Phosphate (ortho-phosphate) Cell Test	1.00673.0001			¹⁾	1.19898.0500
Phosphate (ortho-phosphate) Cell Test	1.14546.0001			¹⁾	1.19898.0500
Phosphate Test (ortho-phosphate)	1.14848.0001 1.14848.0002	1.14676.0001		¹⁾	1.19898.0500
Phosphate Test (ortho-phosphate)	1.00798.0001			¹⁾	1.19898.0500
Phosphate Test (ortho-phosphate)	1.14842.0001			¹⁾	1.19898.0500
Potassium Cell Test	1.14562.0001			¹⁾	1.70230.0100
Potassium Cell Test	1.00615.0001			¹⁾	1.70230.0100
R Residual Hardness Cell Test	1.14683.0001			¹⁾	1.19778.0100
S Silicate (silicic acid) Test	1.01813.0001		1.32244.0100	¹⁾	1.70236.0100
Silicate (silicic acid) Test	1.14794.0001			¹⁾	1.70236.0100
Silicate (silicic acid) Test	1.00857.0001			¹⁾	1.70236.0100
Silver Test	1.14831.0001			¹⁾	1.19797.0100
Sodium Cell Test	1.00885.0001			²⁾	1.19897.0500
Sulfate Cell Test	1.14548.0001	1.14676.0001	1.25050.0100 1.25051.0100	¹⁾	1.19813.0500
Sulfate Cell Test	1.00617.0001	1.14676.0001	1.25051.0100 1.25052.0100	¹⁾	1.19813.0500

¹⁾ Standard solution, ready-to-use, 1,000 mg/L analyt. Traceable to SRM of NIST (see Ord. No. Certipur® standard solution) | ²⁾ Own standards. Worksheets how to prepare these standards can be downloaded from our website www.merckmillipore.com/aaf > Photometry > Field of Activity/Sample = Standard | ³⁾ For photometers of other manufacturers

Parameters S-Z

Test kit	Ord. No. Test kit	Ord. No. CombiCheck	Ord. No. Standard solution, CRM	Alternative Standard	Ord. No. Certipur® standard sol.
S	Sulfate Cell Test	1.14564.0001	1.14675.0001	1.25051.0100 1.25052.0100 1.25053.0100	¹⁾ 1.19813.0500
	Sulfate Cell Test	1.02532.0001		¹⁾	1.19813.0500
	Sulfate Test	1.02537.0001 1.02537.0002	1.14676.0001	1.25050.0100 1.25051.0100	¹⁾ 1.19813.0500
	Sulfate Test	1.01812.0001		¹⁾	1.19813.0500
	Sulfate Test	1.14791.0001	1.14676.0001	1.25050.0100 1.25051.0100	¹⁾ 1.19813.0500
	Sulfide Test	1.14779.0001		²⁾	
	Sulfite Cell Test	1.14394.0001		²⁾	
	Sulfite Test	1.01746.0001		²⁾	
	Surfactants (anionic) Cell Test	1.02552.0001		²⁾	
	Surfactants (cationic) Cell Test	1.01764.0001		1102974 ²⁾	
	Surfactants (nonionic) Cell Test	1.01787.0001		1.33022.0100 1.33023.0100	²⁾
T	Tin Cell Test	1.14622.0001		²⁾	1.70242.0100
	TOC Cell Test	1.14878.0001		1.32247.0100 1.32248.0100 1.32249.0100	¹⁾ 1.09017.0100
	TOC Cell Test	1.14879.0001		1.32251.0100 1.32252.0100 1.32253.0100	¹⁾ 1.09017.0100
	Total Hardness Cell Test	1.00961.0001		NIST3109A ²⁾	
	Total Nitrogen Cell Test	1.00613.0001	1.14695.0001	1.25043.0100 1.25044.0100	²⁾
	Total Nitrogen Cell Test	1.14537.0001	1.14695.0001	1.25043.0100 1.25044.0100	²⁾
	Total Nitrogen Cell Test	1.14763.0001	1.14689.0001	1.25044.0100 1.25045.0100	²⁾
	Volatile Organic Acid Cell Test	1.01749.0001		²⁾	
	Volatile Organic Acid Test	1.01809.0001		²⁾	
	Zinc Cell Test	1.00861.0001	1.18701.0001	¹⁾	1.19806.0100
Z	Zinc Cell Test	1.14566.0001		¹⁾	1.19806.0100
	Zinc Test	1.14832.0001	1.18701.0001	¹⁾	1.19806.0100



Visit our E-shop

All our products for water, food and environmental analytics are available online – day or night. For further details and easy shopping, please visit www.sigma-aldrich.com

Spectroquant® CombiCheck Analytical Quality Assurance

CombiCheck contains multi-parameter standard solutions for checking the overall system – from test kits and instruments to individual working procedures. Each pack contains one standard solution and one addition solution, both of which are directly traceable to NIST primary standards.

When the specified concentration of the standard solution is achieved, the entire analysis system is in order. If there are deviations from the stated value, use the addition solution to identify errors due to interfering substances in the sample matrix. In case the recovery rate is insufficient (beyond specified tolerances), analyze and eliminate the cause through appropriate countermeasures, such as sample pre-treatment.

CombiCheck **10**

Ord. No. 1.14676.0001 Spectroquant® CombiCheck 10

	Parameter	Concentration and working tolerance	can be used for test kits Ord. No.	Standard solution [mL]	Number of quality checks
Standard Solution Reagent R-1	Ammonium	4.00 ±0.30 mg/L NH ₄ -N	1.14558.0001	1.0	96
	Chloride	25 ±6 mg/L Cl	1.14730.0001	1.0	96
	COD	80 ±12 mg/L COD	1.14540.0001	3.0	32
		80 ±12 mg/L COD	1.18751.0001	2.0	48
	Nitrate	2.50 ±0.25 mg/L NO ₃ -N	1.14556.0001	2.0	48
		2.50 ±0.25 mg/L NO ₃ -N	1.14773.0001 ²⁾	1.5	64
		2.50 ±0.25 mg/L NO ₃ -N	1.09713.0001 ³⁾	1.0	96
	Phosphate ⁴⁾	0.80 ±0.08 mg/L PO ₄ -P	1.00474.0001	5.0	19
		0.80 ±0.08 mg/L PO ₄ -P	1.14543.0001	5.0	19
		0.80 ±0.08 mg/L PO ₄ -P	1.14848.0001/ .0002 ²⁾	5.0	19
		0.80 ±0.08 mg/L PO ₄ -P	1.14848.0001 ³⁾ / .0002 ³⁾	10.0	9
	Sulfate	100 ±15 mg/L SO ₄ ²⁻	1.14548.0001	5.0	19
		100 ±15 mg/L SO ₄ ²⁻	1.00617.0001	2.0	48
		100 ±15 mg/L SO ₄ ²⁻	1.14791.0001	2.5	38
		100 ±15 mg/L SO ₄ ²⁻	1.02537.0001	5.0	19
Addition Solution Reagent R-2 (for spiking of samples)	Ammonium	3.00 ±0.25 mg/L NH ₄ -N	1.14558.0001	0.10	280
	Chloride	25 ±6 mg/L Cl	1.14730.0001	0.10	280
	COD	30 ±8 mg/L COD	1.14540.0001	0.10	280
		45 ±8 mg/L COD	1.18751.0001	0.10	280
	Nitrate	1.50 ±0.20 mg/L NO ₃ -N	1.14556.0001	0.10	280
		2.00 ±0.40 mg/L NO ₃ -N	1.14773.0001 ²⁾	0.10	280
		3.00 ±0.50 mg/L NO ₃ -N	1.09713.0001 ³⁾	0.10	280
		6.0 ±1.0 mg/L NO ₃ -N	1.09713.0001 ¹⁾ ²⁾	0.10	280
	Phosphate ⁴⁾	0.60 ±0.07 mg/L PO ₄ -P	1.00474.0001	0.10	280
		0.60 ±0.07 mg/L PO ₄ -P	1.14543.0001	0.10	280
		0.30 ±0.05 mg/L PO ₄ -P	1.14848.0001/ .0002 ³⁾	0.10	280
	Sulfate	40 ±5 mg/L SO ₄ ²⁻	1.14548.0001	0.10	280
		100 ±15 mg/L SO ₄ ²⁻	1.00617.0001	0.10	280
		80 ±10 mg/L SO ₄ ²⁻	1.14791.0001 ¹⁾	0.10	280
		40 ±5 mg/L SO ₄ ²⁻	1.02537.0001	0.10	280

¹⁾ using a 10-mm rectangular cell, Ord. No. 1.14946.0001

²⁾ using a 20-mm rectangular cell, Ord. No. 1.14947.0001

³⁾ using a 50-mm rectangular cell, Ord. No. 1.14944.0001

⁴⁾ only the determination of ortho-phosphate can be checked



CombiCheck 20

Spectroquant® CombiCheck 20

Ord. No. 1.14675.0001

Parameter	Concentration and working tolerance	can be used for test kits Ord. No.	Standard solution [mL]	Number of quality checks	
Ammonium	12.0 ±1.0 mg/L NH ₄ -N	1.14544.0001	0.50	192	Standard Solution Reagent R-1
Chloride	60 ±10 mg/L Cl	1.14730.0001	1.0	96	
COD	750 ±75 mg/L COD	1.14541.0001	3.0	32	
	750 ±75 mg/L COD	1.18752.0001	2.0	48	
Nitrate	9.0 ±0.9 mg/L NO ₃ -N	1.14563.0001	1.0	96	
	9.0 ±0.9 mg/L NO ₃ -N	1.14542.0001	1.5	64	
	9.0 ±0.9 mg/L NO ₃ -N	1.09713.0001/ .0002 ¹⁾	0.50	192 ¹⁾	
	9.0 ±0.9 mg/L NO ₃ -N	1.14773.0001 ¹⁾	1.5	64	
	9.0 ±0.9 mg/L NO ₃ -N	1.14942.0001	1.0	96	
Phosphate ⁴⁾	8.0 ±0.7 mg/L PO ₄ -P	1.00475.0001	1.0	96	Addition Solution Reagent R-2 (for spiking of samples)
	8.0 ±0.7 mg/L PO ₄ -P	1.14729.0001	1.0	96	
Sulfate	500 ±75 mg/L SO ₄ ²⁻	1.14564.0001	1.0	96	
Ammonium	8.0 ±0.8 mg/L NH ₄ -N	1.14544.0001	0.10	280	
Chloride	40 ±7 mg/L Cl	1.14730.0001	0.10	280	
COD	200 ±40 mg/L COD	1.14541.0001	0.10	280	
	300 ±40 mg/L COD	1.18752.0001	0.10	280	
Nitrate	7.5 ±0.8 mg/L NO ₃ -N	1.14563.0001	0.10	280	
	5.0 ±0.6 mg/L NO ₃ -N	1.14542.0001	0.10	280	
	15.0 ±1.5 mg/L NO ₃ -N	1.09713.0001/ .0002	0.10	280	
	5.0 ±0.6 mg/L NO ₃ -N	1.14773.0001 ¹⁾	0.10	280	
	7.5 ±0.8 mg/L NO ₃ -N	1.14942.0001 ¹⁾	0.10	280	
Phosphate ⁴⁾	5.0 ±0.5 mg/L PO ₄ -P	1.00475.0001	0.10	280	
	5.0 ±0.5 mg/L PO ₄ -P	1.14729.0001	0.10	280	
Sulfate	150 ±30 mg/L SO ₄ ²⁻	1.14564.0001	0.10	280	

CombiCheck 50

Spectroquant® CombiCheck 50

Ord. No. 1.14695.0001

Parameter	Concentration and working tolerance	can be used for test kits Ord. No.	Standard solution [mL]	Number of quality checks	
Ammonium	1.000 ±0.100 mg/L NH ₄ -N	1.14739.0001	5.0	19	Standard Solution Reagent R-1
	1.00 ±0.10 mg/L NH ₄ -N	1.14752.0002/ .0001 ¹⁾	5.0	19	
COD	20.0 ±4.0 mg/L COD	1.14560.0001	3.0	32	
	20.0 ±4.0 mg/L COD	1.01796.0001	2.0	48	Addition Solution Reagent R-2 (for spiking of samples)
	20.0 ±4.0 mg/L COD	1.18750.0001	2.0	48	
Nitrogen	5.0 ±0.7 mg/L N	1.00613.0001	10	9	
	5.0 ±0.7 mg/L N	1.14537.0001	10	9	
Ammonium	1.000 ±0.100 mg/L NH ₄ -N	1.14739.0001	0.10	280	
	1.00 ±0.10 mg/L NH ₄ -N	1.14752.0002/ .0001 ¹⁾	0.10	280	
COD	10.0 ±3.0 mg/L COD	1.14560.0001	0.10	280	
	15.0 ±3.0 mg/L COD	1.01796.0001	0.10	280	
	15.0 ±3.0 mg/L COD	1.18750.0001	0.10	280	
Nitrogen	3.0 ±0.5 mg/L N	1.00613.0001	0.10	280	
	3.0 ±0.5 mg/L N	1.14537.0001	0.10	280	

Spectroquant® CombiCheck Analytical Quality Assurance

CombiCheck 60

Ord. No. 1.14696.0001

Spectroquant® CombiCheck 60

	Parameter	Concentration and working tolerance	can be used for test kits Ord. No.	Standard solution [mL]	Number of quality checks
Standard Solution Reagent R-1	Chloride	125 ±13 mg/L Cl ⁻	1.14897.0001/ .0002	1.0	96
	COD	250 ±25 mg/L COD	1.14690.0001	2.0	48
		250 ±20 mg/L COD	1.14895.0001	2.0	48
Addition Solution Reagent R-2 (for spiking of samples)	Chloride	50 ±7 mg/L Cl ⁻	1.14897.0001/ .0002	0.10	280
	COD	75 ±15 mg/L COD	1.14690.0001	0.10	280
		75 ±10 mg/L COD	1.14895.0001	0.10	280

CombiCheck 70

Ord. No. 1.14689.0001

Spectroquant® CombiCheck 70

	Parameter	Concentration and working tolerance	can be used for test kits Ord. No.	Standard solution [mL]	Number of quality checks
Standard Solution Reagent R-1	Ammonium	50.0 ±5.0 mg/L NH ₄ -N	1.14559.0001	0.10	960
	Ammonium (2.0 – 75.0 mg/L)	50.0 ±5.0 mg/L NH ₄ -N	1.00683.0001 ^{1) 5)}	0.20	480
	Ammonium (5 – 150 mg/L)	50 ±5 mg/L NH ₄ -N	1.00683.0001 ^{1) 5)}	0.10	960
	COD	5,000 ±400 mg/L COD	1.14555.0001	1.0	96
		5,000 ±400 mg/L COD	1.18753.0001	0.20	480
	Nitrogen	50 ±7 mg/L N	1.14763.0001	1.0	96
Addition Solution Reagent R-2 (for spiking of samples)	Ammonium	20.0 ±2.0 mg/L NH ₄ -N	1.14559.0001	0.10	280
	Ammonium (2.0 – 75.0 mg/L)	10.0 ±1.0 mg/L NH ₄ -N	1.00683.0001 ^{1) 5)}	0.10	280
	Ammonium (5 – 150 mg/L)	20 ±2 mg/L NH ₄ -N	1.00683.0001 ^{1) 5)}	0.10	280
	COD	2,000 ±200 mg/L COD	1.14555.0001	0.10	280
	Nitrogen	20 ±6 mg/L N	1.14763.0001	0.10	280

CombiCheck 80

Ord. No. 1.14738.0001

Spectroquant® CombiCheck 80

	Parameter	Concentration and working tolerance	can be used for test kits Ord. No.	Standard solution [mL]	Number of quality checks
Standard Solution Reagent R-1	COD	1,500 ±150 mg/L COD	1.14691.0001	2.0	48
	Nitrate	25.0 ±2.5 mg/L NO ₃ -N	1.14764.0001	0.50	190
	Phosphate ⁴⁾	15.0 ±1.0 mg/L PO ₄ -P	1.00475.0001	1.0	96
		15.0 ±1.0 mg/L PO ₄ -P	1.14729.0001	1.0	96
Addition Solution Reagent R-2 (for spiking of samples)	COD	1,000 ±100 mg/L COD	1.14691.0001	0.10	280
	Nitrate	10.0 ±1.5 mg/L NO ₃ -N	1.14764.0001	0.10	280
	Phosphate ⁴⁾	5.0 ±0.5 mg/L PO ₄ -P	1.00475.0001	0.10	280
		5.0 ±0.5 mg/L PO ₄ -P	1.14729.0001	0.10	280

1) using a 10-mm rectangular cell, Ord. No. 1.14946.0001

2) using a 20-mm rectangular cell, Ord. No. 1.14947.0001

3) using a 50-mm rectangular cell, Ord. No. 1.14944.0001

4) only the determination of ortho-phosphate can be checked

5) when using AutoSelector, measuring range 5 - 150 mg/L NH₄-N is used

CombiCheck 90

Spectroquant® CombiCheck 90

Ord. No. 1.18700.0001

Parameter	Concentration and working tolerance	can be used for test kits Ord. No.	Standard solution [mL]	Number of quality checks	
Cadmium	0.250 ±0.030 mg/L Cd	1.01745.0001 ¹⁾	10.0	9	Standard Solution Reagent R-1
	0.250 ±0.030 mg/L Cd	1.14834.0001	5.0	19	
Iron	1.00 ±0.15 mg/L Fe	1.14549.0001	5.0	19	
	1.00 ±0.15 mg/L Fe	1.14761.0001 ¹⁾	5.0	19	
	1.00 ±0.15 mg/L Fe	1.00796.0001 ¹⁾	8.0	12	
Copper	2.00 ±0.20 mg/L Cu	1.14553.0001	5.0	19	
	2.00 ±0.20 mg/L Cu	1.14767.0001 ¹⁾	5.0	19	
Manganese	1.00 ±0.15 mg/L Mn	1.00816.0001	7.0	13	Addition Solution Reagent R-2 (for spiking of samples)
	1.00 ±0.15 mg/L Mn	1.14770.0001 ³⁾	10.0	9	
	1.00 ±0.15 mg/L Mn	1.01846.0001 ¹⁾	8.0	12	
Cadmium	0.100 ±0.015 mg/L Cd	1.01745.0001 ¹⁾	0.10	280	
	0.200 ±0.030 mg/L Cd	1.14834.0001	0.10	280	
Iron	3.00 ±0.30 mg/L Fe	1.14549.0001	0.10	280	
	3.00 ±0.30 mg/L Fe	1.14761.0001 ¹⁾	0.10	280	
	1.88 ±0.20 mg/L Fe	1.00796.0001 ¹⁾	0.10	280	
Copper	3.00 ±0.30 mg/L Cu	1.14553.0001	0.10	280	
	3.00 ±0.30 mg/L Cu	1.14767.0001 ¹⁾	0.10	280	
Manganese	1.43 ±0.15 mg/L Mn	1.00816.0001	0.10	280	
	1.00 ±0.15 mg/L Mn	1.14770.0001 ³⁾	0.10	280	
	1.25 ±0.15 mg/L Mn	1.01846.0001 ¹⁾	0.10	280	

CombiCheck 100

Spectroquant® CombiCheck 100

Ord. No. 1.18701.0001

Parameter	Concentration and working tolerance	can be used for test kits Ord. No.	Standard solution [mL]	Number of quality checks	
Aluminium	0.40 ±0.05 mg/L Al	1.00594.0001	6.0	16	Standard Solution Reagent R-1
	0.40 ±0.05 mg/L Al	1.14825.0001 ¹⁾	5.0	19	
Lead	2.00 ±0.20 mg/L Pb	1.14833.0001	5.0	19	Addition Solution Reagent R-2 (for spiking of samples)
	2.00 ±0.20 mg/L Pb	1.09717.0001 ¹⁾	8.0	11	
Nickel	2.00 ±0.20 mg/L Ni	1.14554.0001	5.0	19	
	2.00 ±0.20 mg/L Ni	1.14785.0001 ¹⁾	5.0	19	
Zinc	0.750 ±0.150 mg/L Zn	1.00861.0001	10.0	9	
	0.75 ±0.15 mg/L Zn	1.14832.0001	5.0	19	
Aluminium	0.20 ±0.03 mg/L Al	1.00594.0001	0.10	280	
	0.24 ±0.04 mg/L Al	1.14825.0001 ¹⁾	0.10	280	
Lead	1.00 ±0.15 mg/L Pb	1.14833.0001	0.10	280	
	0.63 ±0.10 mg/L Pb	1.09717.0001 ¹⁾	0.10	280	
Nickel	2.00 ±0.20 mg/L Ni	1.14554.0001	0.10	280	
	2.00 ±0.20 mg/L Ni	1.14785.0001 ¹⁾	0.10	280	
Zinc	0.250 ±0.050 mg/L Zn	1.00861.0001	0.10	280	
	0.50 ±0.10 mg/L Zn	1.14832.0001	0.10	280	

Certified Reference Materials
for photometric applications

NO DILUTION.
NO DOUBTS.
NO DELAYS.

PRECISE
ANALYTICAL
QUALITY
CONTROL

NO DILUTION
NEEDED


DIRECTLY
TRACEABLE
TO NIST

Exact, batch-specific concentration,
and expanded measurement uncertainty

Also see our

Krom et al.
CRM s (page 107)

Experience absolute precision in photometric quality control with our ready-to-use diluted certified reference materials (CRMs). Thanks to their exact concentrations, expanded measurement uncertainty, and direct traceability to NIST primary reference materials, our CRMs ensure that your results are correct and comparable worldwide.

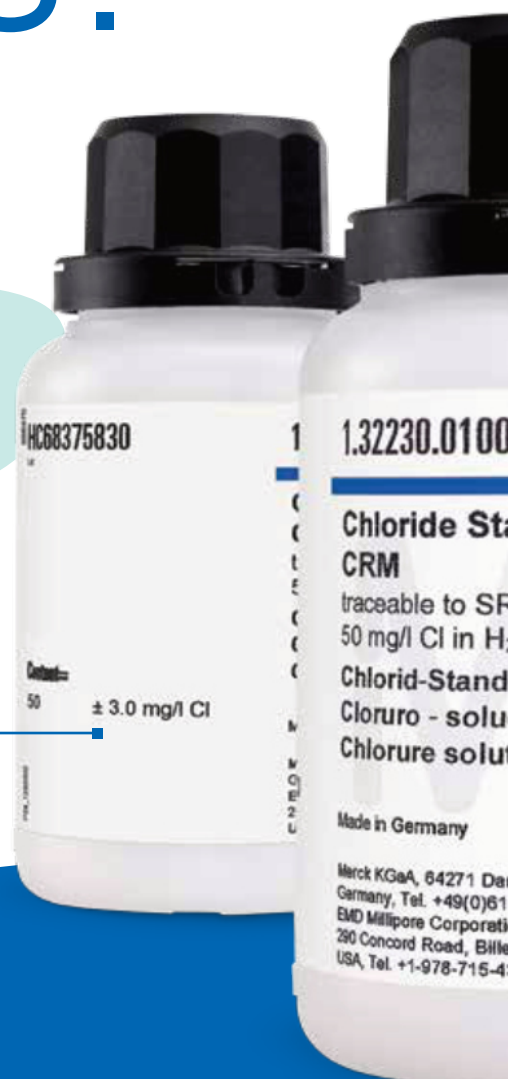

Complete range with all parameters for analytical quality control of wastewater, drinking water and process water

Detailed Certificate of Analysis for each CRM simplifies accreditation

Compatible with Spectroquant® test kits or those from other suppliers

Ready-to-use, diluted CRMs save time and prevent dilution errors

Long shelf life of 24 months

Directly traceable to NIST primary measurement standards

Ideal for validating international norm methods: ISO, EN, EPHA, and EPA

Even better together

The perfect combination for water analysis: use our certified standard solutions with Spectroquant® Prove spectrophotometers.

Learn more about:
Prove (page 36) and CRMs (page 104)

Definitions

Traceability

"Property of a measurement result whereby the result can be related to a reference through a documented unbroken chain of calibrations, each contributing to the measurement uncertainty."¹⁾

Certified reference material (CRM)

"Reference material (RM) characterized by a metrologically valid procedure for one or more specified properties, accompanied by an RM certificate that provides the value of the specified property, its associated uncertainty, and a statement of metrological traceability."²⁾

Primary measurement standard


"Measurement standard that is designated or widely acknowledged as having the highest metrological qualities and whose property value is accepted without reference to other standards of the same property or quantity, within a specified context."²⁾

Secondary measurement standard

"Measurement standard whose property value is assigned by comparison with a primary measurement standard of the same property or quantity."²⁾

¹⁾ ISO Guide 99:2007; *International Vocabulary of Metrology – Basic and General Concepts and Associated Terms (VIM)*

²⁾ ISO/Guide 30:2015; *Reference Materials – Selected Terms and Definitions*

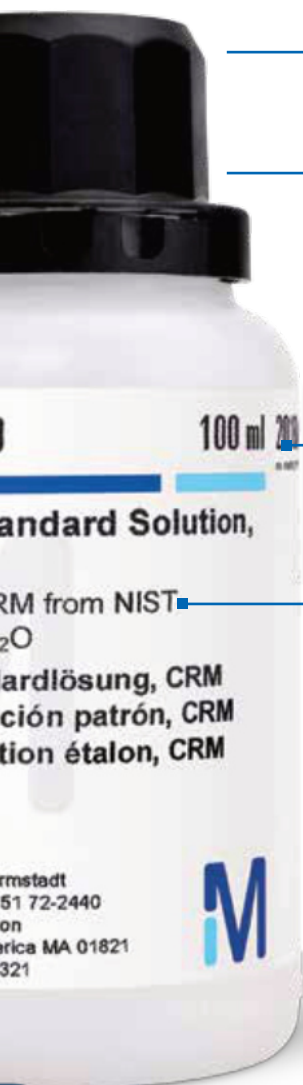

Certified Reference Materials for photometric applications

Standard Solutions (100 mL in H₂O), traceable to SRM from NIST

	Product	Concentration	Expanded Measurement Uncertainty	Ord. No.
A	Aluminium Standard Solution	0.0500 mg/L Al	± 0.0020 mg/L Al	1.32226.0100
	Aluminium Standard Solution	0.200 mg/L Al	± 0.006 mg/L Al	1.32225.0100
	Ammonium Standard Solution	0.250 mg/L NH ₄	± 0.011 mg/L NH ₄	1.32227.0100
	Ammonium Standard Solution	0.400 mg/L NH ₄ -N	± 0.012 mg/L NH ₄ -N	1.25022.0100
	Ammonium Standard Solution	1.00 mg/L NH ₄ -N	± 0.04 mg/L NH ₄ -N	1.25023.0100
	Ammonium Standard Solution	2.00 mg/L NH ₄ -N	± 0.07 mg/L NH ₄ -N	1.25024.0100
	Ammonium Standard Solution	6.00 mg/L NH ₄ -N	± 0.13 mg/L NH ₄ -N	1.25025.0100
	Ammonium Standard Solution	12.0 mg/L NH ₄ -N	± 0.4 mg/L NH ₄ -N	1.25026.0100
	Ammonium Standard Solution	50.0 mg/L NH ₄ -N	± 1.2 mg/L NH ₄ -N	1.25027.0100
	Arsenic Standard Solution	1.00 mg/L As	± 0.05 mg/L As	1.33002.0250 ^{1) 2)}
B	Boron Standard Solution	1.00 mg/L B	± 0.06 mg/L B	1.33005.0100
	Bromate Standard Solution	0.0100 mg/L BrO ₃	± 0.0006 mg/L BrO ₃	1.33006.0100
	Bromate Standard Solution	0.1000 mg/L BrO ₃	± 0.0040 mg/L BrO ₃	1.33007.0100
C	Cadmium Standard Solution	0.00500 mg/L Cd	± 0.00020 mg/L Cd	1.33008.0100 ¹⁾
	Cadmium Standard Solution	0.100 mg/L Cd	± 0.003 mg/L Cd	1.32228.0100
	Chloride Standard Solution	0.100 mg/L Cl	± 0.006 mg/L Cl ⁻	1.33009.0100
	Chloride Standard Solution	1.00 mg/L Cl	± 0.04 mg/L Cl ⁻	1.33010.0100
	Chloride Standard Solution	2.50 mg/L Cl	± 0.08 mg/L Cl ⁻	1.33011.0100
	Chloride Standard Solution	10.0 mg/L Cl	± 0.5 mg/L Cl ⁻	1.32229.0100
	Chloride Standard Solution	50 mg/L Cl	± 3 mg/L Cl ⁻	1.32230.0100
	Chloride Standard Solution	250 mg/L Cl	± 8 mg/L Cl ⁻	1.32231.0100
	Chromium Standard Solution	0.050 mg/L Cr(VI)	± 0.002 mg/L Cr(VI)	1.33012.0100
	Chromium Standard Solution	1.00 mg/L Cr(VI)	± 0.03 mg/L Cr(VI)	1.33013.0100
	COD Standard Solution	20.0 mg/L	± 0.7 mg/L	1.25028.0100
	COD Standard Solution	100 mg/L	± 3 mg/L	1.25029.0100
	COD Standard Solution	200 mg/L	± 4 mg/L	1.25030.0100
	COD Standard Solution	400 mg/L	± 5 mg/L	1.25031.0100
	COD Standard Solution	1,000 mg/L	± 11 mg/L	1.25032.0100
	COD Standard Solution	2,000 mg/L	± 32 mg/L	1.25033.0100
	COD Standard Solution	8,000 mg/L	± 68 mg/L	1.25034.0100
	COD Standard Solution	50,000 mg/L	± 894 mg/L	1.25035.0100
F	Fluoride Standard Solution	0.200 mg/L F	± 0.012 mg/L F	1.32234.0100
	Fluoride Standard Solution	0.50 mg/L F	± 0.02 mg/L F	1.32233.0100
	Fluoride Standard Solution	1.00 mg/L F	± 0.03 mg/L F	1.32235.0100
	Fluoride Standard Solution	1.50 mg/L F	± 0.04 mg/L F	1.32236.0100
I	Iron Standard Solution	0.0500 mg/L Fe	± 0.0015 mg/L Fe	1.33014.0100 ¹⁾
	Iron Standard Solution	0.1000 mg/L Fe	± 0.0030 mg/L Fe	1.33018.0100 ¹⁾
	Iron Standard Solution	0.300 mg/L Fe	± 0.009 mg/L Fe	1.33019.0100 ¹⁾
	Iron Standard Solution	1.00 mg/L Fe	± 0.04 mg/L Fe	1.33020.0100 ¹⁾
L	Lead Standard Solution	0.0500 mg/L Pb	± 0.0040 mg/L Pb	1.33003.0100 ¹⁾
	Lead Standard Solution	0.100 mg/L Pb	± 0.005 mg/L Pb	1.33004.0100 ¹⁾
M	Manganese Standard Solution	0.050 mg/L Mn	± 0.004 mg/L Mn	1.32237.0100
	Manganese Standard Solution	0.200 mg/L Mn	± 0.005 mg/L Mn	1.32238.0100
	Manganese Standard Solution	1.00 mg/L Mn	± 0.03 mg/L Mn	1.32239.0100

Standard Solutions (100 mL in H₂O), traceable to SRM from NIST

	Product	Concentration	Expanded Measurement Uncertainty	Ord. No.
N	Nitrate Standard Solution	1.00 mg/L NO ₃	± 0.03 mg/L NO ₃	1.32240.0100
	Nitrate Standard Solution	10.0 mg/L NO ₃	± 0.3 mg/L NO ₃	1.32241.0100
	Nitrate Standard Solution	50.0 mg/L NO ₃	± 2.0 mg/L NO ₃	1.32242.0100
	Nitrate Standard Solution	0.50 mg/L NO ₃ -N	± 0.05 mg/L NO ₃ -N	1.25036.0100
	Nitrate Standard Solution	2.50 mg/L NO ₃ -N	± 0.06 mg/L NO ₃ -N	1.25037.0100
	Nitrate Standard Solution	15.0 mg/L NO ₃ -N	± 0.4 mg/L NO ₃ -N	1.25038.0100
	Nitrate Standard Solution	40.0 mg/L NO ₃ -N	± 1 mg/L NO ₃ -N	1.25039.0100
	Nitrate Standard Solution	200 mg/L NO ₃ -N	± 5 mg/L NO ₃ -N	1.25040.0100
	Nitrite Standard Solution	0.0100 mg/L NO ₂ ⁻	± 0.0012 mg/L NO ₂ ⁻	1.33021.0100 ³⁾
	Nitrite Standard Solution	0.200 mg/L NO ₂ -N	± 0.009 mg/L NO ₂ -N	1.25041.0100
	Nitrite Standard Solution	40.0 mg/L NO ₂ -N	± 1.3 mg/L NO ₂ -N	1.25042.0100
	Nitrogen (total) Standard Solution	2.50 mg/L N	± 0.06 mg/L N	1.25043.0100
	Nitrogen (total) Standard Solution	12.0 mg/L N	± 0.3 mg/L N	1.25044.0100
	Nitrogen (total) Standard Solution	100 mg/L N	± 3 mg/L N	1.25045.0100
P	Phosphorus Standard Solution	0.400 mg/L PO ₄ -P	± 0.016 mg/L PO ₄ -P	1.25046.0100
	Phosphorus Standard Solution	4.00 mg/L PO ₄ -P	± 0.08 mg/L PO ₄ -P	1.25047.0100
	Phosphorus Standard Solution	15.0 mg/L PO ₄ -P	± 0.4 mg/L PO ₄ -P	1.25048.0100
	Phosphorus Standard Solution	75.0 mg/L PO ₄ -P	± 1.6 mg/L PO ₄ -P	1.25049.0100
S	Silicate Standard Solution	0.1000 mg/L SiO ₂	± 0.0040 mg/L SiO ₂	1.32244.0100
	Silicate Standard Solution	0.500 mg/L SiO ₂	± 0.025 mg/L SiO ₂	1.32243.0100
	Silicate Standard Solution	1.000 mg/L SiO ₂	± 0.030 mg/L SiO ₂	1.32245.0100
	Sulfate Standard Solution	40 mg/L SO ₄	± 6 mg/L SO ₄	1.25050.0100
	Sulfate Standard Solution	125 mg/L SO ₄	± 6 mg/L SO ₄	1.25051.0100
	Sulfate Standard Solution	400 mg/L SO ₄	± 20 mg/L SO ₄	1.25052.0100
	Sulfate Standard Solution	800 mg/L SO ₄	± 27 mg/L SO ₄	1.25053.0100
	Surfactants (nonionic) Standard Solution ⁴⁾	1.00 mg/L Triton® X-100	± 0.16 mg/L Triton® X-100	1.33022.0100
	Surfactants (nonionic) Standard Solution ⁴⁾	5.00 mg/L Triton® X-100	± 0.30 mg/L Triton® X-100	1.33023.0100
	Surfactants (nonionic) Standard Solution ⁴⁾	10.00 mg/L Triton® X-100	± 0.30 mg/L Triton® X-100	1.33024.0100
T	TOC Standard Solution	5.00 mg/L TOC	± 0.10 mg/L TOC	1.32246.0100
	TOC Standard Solution	10.0 mg/L TOC	± 0.2 mg/L TOC	1.32247.0100
	TOC Standard Solution	25.0 mg/L TOC	± 0.5 mg/L TOC	1.32248.0100
	TOC Standard Solution	50.0 mg/L TOC	± 1.0 mg/L TOC	1.32249.0100
	TOC Standard Solution	100 mg/L TOC	± 2 mg/L TOC	1.32251.0100
	TOC Standard Solution	200 mg/L TOC	± 4 mg/L TOC	1.32252.0100
	TOC Standard Solution	500 mg/L TOC	± 10 mg/L TOC	1.32253.0100

1) 100 mL in HNO₃ 2) 250 mL bottle 3) 100 mL in NaOH 4) traceable to USP

FREE COA

Certificates of Analysis (COA) for all our standard solutions can be downloaded free of charge on:
www.merckmillipore.com/coa



Certipur® standard solutions

Parameters A-Z

Certipur® standard solutions, concentration 1,000 mg/L

Certipur® standard solutions are **traceable to standard reference materials from NIST**, and accredited according to ISO/IEC 17025 guidelines. They can be easily diluted to different concentrations to suit your needs.

Parameter	Volume	Ord. No.	Parameter	Volume	Ord. No.
A Aluminium	100 mL	1.19770.0100	N Nickel*	1,000 mL	1.09989.0001
Ammonium	500 mL	1.19812.0500	Nitrate	500 mL	1.19811.0500
Antimony	100 mL	1.70204.0100	Nitrite	500 mL	1.19899.0500
Arsenic	100 mL	1.19773.0100	P Palladium	100 mL	1.14282.0100
B Boron	100 mL	1.19500.0100	Phosphate	500 mL	1.19898.0500
C Cadmium	100 mL	1.19777.0100	Platinum	100 mL	1.70219.0100
Calcium	100 mL	1.19778.0100	Potassium	100 mL	1.70230.0100
Chloride	500 mL	1.19897.0500	S Silicon	100 mL	1.70236.0100
Chromate	500 mL	1.19780.0500	Silver	100 mL	1.19797.0100
Chromium	100 mL	1.19779.0100	Sulfate	500 mL	1.19813.0500
Cobalt	100 mL	1.19785.0100	T Tin	100 mL	1.70242.0100
Copper	100 mL	1.19786.0100	TOC	100 mL	1.09017.0100
Cyanide	500 mL	1.19533.0500	V Vanadium	100 mL	1.70245.0100
F Fluoride	500 mL	1.19814.0500	Z Zinc	100 mL	1.19806.0100
G Gold	100 mL	1.70216.0100	* Titrisol®		
I Iron	100 mL	1.19781.0100			
L Lead	100 mL	1.19776.0100			
M Magnesium	100 mL	1.19788.0100			
Manganese	100 mL	1.19789.0100			
Mercury	100 mL	1.70226.0100			
Molybdenum	100 mL	1.70227.0100			



Proficiency testing (PT) process

- 1. Registration & order** – Prior to your first order, you must obtain a lab code by registering on the PT portal.
- 2. Delivery** – Participating labs receive blind samples according to schedule.
- 3. Open study** – Each lab analyzes the blind samples.
- 4. Reporting** – Labs report results on the PT portal before the study closes.
- 5. Data processing** – Data is processed to issue individual evaluation reports.
- 6. Evaluation report** – Reports are sent via the PT portal. If requested, a copy is sent to your accreditation body.

Proficiency testing products

Proficiency testing products accredited by ACLASS to ISO/IEC 17043:2010, Certificate No. AP-1469 and recognized by accreditation bodies worldwide

Application fields	Metals and Inorganics	Organics	Gases	Physical Properties
Drinking Water	■	■		■
Wastewater	■	■		■
Contaminated Land	■	■		
Air Quality and Emissions	■	■	■	
Microbiology		■		

Certified Reference Materials for instrument qualification

Kromega CRMs for UV/Vis spectrophotometers

Ready-to-use Kromega certified reference materials are designed to facilitate qualification of UV/Vis spectrophotometers for compliance with GLP regulations.

- Meet European Pharmacopoeia requirements for the calibration of UV/Vis spectrophotometers
- Reliable, traceable instrument qualification with audit trail supported by independent verification according to ISO Guide 34
- Easier, faster and more cost-effective than custom solutions
- Developed for use in any laboratory working according to ISO 17025
- Shipped in flame-sealed ampoules, and protected in custom-made boxes to increase shelf life and prevent contamination

Learn more about Kromega CRMs:

www.sigmaaldrich.com/jaytee



CRMs for photometers

Product	Description	Content	Cat. No.
UV Photometric Accuracy Standards	Used to qualify photometric accuracy of UV spectrophotometers to the limits defined in the EP	3 ampoules (1 blank, 2 standards). The standards consist of a solution of $K_2Cr_2O_7$ in Perchloric Acid	Z804452
UV Resolution Standards	Used to qualify the UV resolution of UV spectrophotometers to the limits defined in the EP	2 ampoules (1 blank, 1 standard). The standard consists of a solution of toluene in n-hexane.	Z804568
UV Stray Light Standards	Used to qualify the stray light of UV spectrophotometers to the limits defined in the EP	2 ampoules (1 blank, 1 standard). The standard consists of a solution of NaCl in water.	Z804665
UV Spec Qualification Kit	To be used in any laboratory regardless of the regulator and are as relevant to a pharmaceutical company as to a contract lab working to ISO 17025.	Contains qualification standards for UV Photometric Accuracy Resolution Stray Light	Z804789

GET CLARITY IN ANY WATER

How clear is your solution?

A perfect solution has no turbidity. But it doesn't exist in reality. That's why the quantification of turbidity is crucial in proficiency testing. It is usually performed to check the efficiency of filtration units, such as in pools and spas, or food and beverage production plants. It is also needed in process control, for example to monitor coagulation in wastewater treatment.

We have the answer

Turbiquant® turbidimeters are designed to simplify turbidity analysis. They offer rapid, reliable measurements in the lab or on-site, and can be combined with our non-toxic calibration standards for safe and clear results. The instruments are available with either an infrared (IR) or tungsten (T) light source. Choose the system that best suits your needs.

IR: Infrared light at 860 nm

- Required in Europe for ISO 7027 or DIN EN 27027
- Less prone to interferences in intensely-colored solutions

T: Tungsten lamp at spectra of visible white light

- Required in the US for Standard Methods 2130 B and USEPA
- Better for measuring turbidity caused by very small particles





Turbidimetry

Turbiquant®

General information	110
Turbiquant® 1100 IR and 1100 T	112
Turbiquant® 1500 T	112
Turbiquant® 3000 IR	113
Turbiquant® calibration standards	113



Cooling & boiler water workflow
> Page 20



Wastewater workflow
> Page 22



Drinking water workflow
> Page 24



Bottled water workflow
> Page 26

Turbiquant®

Get clarity in any water

What is turbidity?

Turbidity is "the decrease in the transparency of a liquid caused by the presence of undissolved substances" (DIN EN 27027). Thus, clear water has a lower turbidity measurement than muddy water containing suspended particles, such as bacteria, sediments or sewage.

How is it measured?

In nephelometric turbidity measurement, entering light is scattered and measured at 90° using a detector. The signals are characteristically non-linear. Thus, samples with very high turbidity, like untreated wastewater, show a decreasing signal with increasing turbidity. For added security, these samples are investigated in transmission (attenuation of translucent light) as well as by classic nephelometry. The combined result is the "NTU ratio".

Clear results with Turbiquant®

Turbiquant® 3000 turbidimeters are ideal for challenging measurements of highly turbid or colored samples. The other Turbiquant® series offer different benefits such as mobility, robustness and compliance with European and/or US standards. Whichever model you choose, you'll always enjoy clear results.



Turbidity is a critical parameter in drinking- and wastewater, beverages, and chemical production.

Typical turbidity values:

Deionized water	0.02 NTU
Drinking water	0.02 to 0.5 NTU
Spring water	0.05 to 10 NTU
Wastewater (untreated)	70 to 2,000 NTU
Sift water (paper industry)	60 to 800 NTU
USEPA	max. level 5 NTU
Japan	max. level 2 NTU
WHO	max. level 5 NTU
France	max. level 4 NTU
Germany	max. level 1 NTU

Incomparable Precision

10 NTU	± 1%
100 NTU	± 1%
1,000 NTU	± 1%
1,750 NTU	± 2%
10,000 NTU	± 2%

M obility

Compact and portable turbidimeter for fast results

Com pliance

Measure samples acc. to EN ISO 7027 or USEPA 180.1

Choice

Tungsten or infrared light source, and a broad range of calibration standards to suit your needs



Need a conductivity meter
or a pH meter?

Find them and more on:
[www.sigmaaldrich.com/labware/
labware-catalog.html](http://www.sigmaaldrich.com/labware/labware-catalog.html)



NTU = Nephelometric Turbidity Units 90° scattered light measurement according to section 2130 of the "Standard Methods for the Examination of Water and Wastewater", 21st edition, 2005.

FNU = Formazine Nephelometric Units 90° scattered light measurement that is only applicable if the instrument is calibrated with Formazine standards. It is used for measurements according to EN ISO 7027 (Conversion: 1 FNU = 1 NTU).

FAU = Formazine Attenuation Units transmission measurement unit for measurements according to EN ISO 7027 over 40 FNU.


EBC = European Brewery Commission 90° scattered light measurement used by the European Brewery Commission (Conversion: 0.245 EBC = 1 NTU).

Turbiquant®

Get clarity in any water



1100

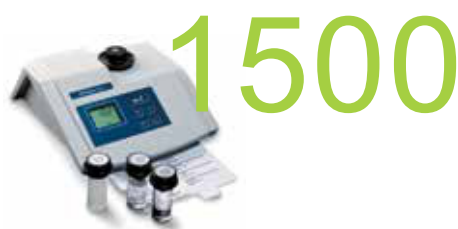

1500

	Turbiquant® 1100 IR (portable)	Turbiquant® 1100 T (portable)	Turbiquant® 1500 T
	Portable instrument for on-the-spot analysis	Portable instrument for on-the-spot analysis	Standard instrument for all applications in the laboratory, suitable for drinking water
Ord. No.	1.18324.0001	1.18325.0001	1.18331.0001
Measuring principle	nephelometric – 90° scattered light, conform with EN ISO 7027	nephelometric – 90° scattered light, follows USEPA recommendations	nephelometric (non ratio), conform with EN ISO 7027 follows USEPA recommendations
Light source	IR LED	white light tungsten lamp	white light tungsten lamp
Indication of units	NTU / FNU	NTU / FNU	NTU / FNU
Measuring range	0.02–1,100 NTU	0.02–1,100 NTU	0.02–1,000 NTU
Resolution	0.01 within the range 0.01 < x < 99.99 NTU 0.1 within the range 100 < x < 999.9 NTU 1 within the range 1,000 < x < 1,100 NTU		max. 0.01 within the range 0 < x < 10 NTU max. 0.1 within the range 10 < x < 100 NTU max. 1 within the range 100 < x < 1,000 NTU
Accuracy	±2 % of reading or ±0.1 NTU for range 0 – 500 NTU ±3 % of reading for range 500 – 1,100 NTU		±2 % of reading or ±0.01 NTU for range 0.00 – 1,000 NTU
Reproducibility	–	–	< ±1% of reading or ±0.01 NTU
Calibration	automatic 1 to 3 points	automatic 1 to 3 points	automatic 1 to 3 points
Response time	14 seconds	14 seconds	< 3 seconds
Cuvettes	25 x 45 mm	25 x 45 mm	28 x 70 mm
Sample volume	15 mL	15 mL	25 mL
Serial input / output	–	–	RS 232, uni-directional
Protection type	designed to meet IP 67	designed to meet IP 67	–
Power requirements	4 alkali manganese batteries, AAA / Micro	4 alkali manganese batteries, AAA / Micro	universal power supply / plug
Test certificates	CE	CE	CE, UL, CSA, TÜV-GS
Warranty	2 years	2 years	2 years
Special features	Portable, battery-operated instrument	Portable, battery-operated instrument	Real time clock integrated GLP function (calibration intervals monitoring), automatic self check

! IR or T? You choose

Infrared (IR) measurements at 860 nm show no interference in colored solutions, and are required by EN ISO 7027. Tungsten (T) lamps emitting white light are more sensitive when measuring small particles, and are required by USEPA 180.1, APHA, AWWA and WPCF.

www.merckmillipore.com/turbidity



Turbiquant® 3000 IR

Precision instrument for demanding turbidimetric applications with very high turbidity and/or colored solutions

1.18332.0001

nephelometric (non-ratio / ratio selectable), conform with EN ISO 7027

IR LED

NTU, FNU, FAU, EBC

0.02–10,000 NTU, 0.02–10,000 FNU, 0.02–10,000 FAU, 0.005–2,450 EBC

selectable 0.1–0.0001 NTU

max. 0.0001 within the range $0 < x < 10$ NTU

max. 0.001 within the range $10 < x < 100$ NTU

max. 0.01 within the range $100 < x < 1,000$ NTU

max. 0.1 within the range $1,000 < x < 10,000$ NTU

±2 % of reading or ±0.01 NTU for range 0.00 – 1,000 NTU

±5 % of reading for range 1,000 – 4,000 NTU

±10 % of reading for range 4,000 – 10,000 NTU

< ±1 % of reading or ±0.01 NTU

automatic 1 to 4 points (to 1,750 NTU) 10,000 NTU selectable

< 6 seconds

28 x 70 mm

25 mL

RS 232, bi-directional

–

universal power supply / plug

CE, UL, CSA, TÜV-GS

2 years

GLP function (calibration interval monitoring), automatic self check, integrated real time clock, safety access codes for calibration and instrument setup

Turbiquant® Calibration Standards

Precise, stable, non-toxic and ready-to-use

Turbiquant® 1100 IR / 1100 T **1.18335.0001**

Calibration Standard Set

3 standards 0.02 – 10.0 – 1,000 NTU

Turbiquant® 1500 IR / 1500 T **1.18328.0001**

Calibration Standard Set

3 standards 0.02 – 10.0 – 1,000 NTU

Turbiquant® 3000 IR **1.18329.0001**

Calibration Standard Set

4 standards 0.02 – 10.0 – 100.0 – 1,750 NTU

Turbiquant® 3000 T **1.18349.0001**

Calibration Standard Set

4 standards 0.02 – 10.0 – 100.0 – 1,750 NTU

Turbiquant® 3000 IR **1.18342.0001**

Calibration Standard

10,000 NTU

Turbiquant® 3000 T **1.18343.0001**

Calibration Standard

10,000 NTU

Turbiquant® 1500 / 3000 **1.18381.0001**

Calibration Standard

10 NTU

Turbiquant® calibration standards can be stored and transported without any precautionary measures. They are supplied with indexing rings for quick, repeatable indexing as recommended by USEPA.



Find more standards for measurements in our section "Environmental Matrix CRMs (RTC)"

! there's more ...

Find Turbiquant® accessories, such as empty cells, and lamps, on: www.merckmillipore.com/turbidity

TAKE YOUR TEST FURTHER

How fresh is your honey?

Rapid quantitative detection of hydroxymethylfurfural in honey

The application

- The freshness of honey is determined by measuring its hydroxymethylfurfural (HMF) content.
- HMF is an organic compound that arises from the dehydration of fructose, e.g. when honey is heated for easier filling.
- HMF is barely detectable in freshly centrifuged honey, but increases at 2-3 mg/kg annually, depending on storage temperature and pH. At 21°C, HMF content can rise to 20 mg/kg in just one year.

Our solution: Reflectoquant® Hydroxymethylfurfural (HMF) Test

The Reflectoquant® HMF Test is the first rapid test for the determination of HMF content, delivering accurate quantitative results in just a few minutes after sample preparation. Easy-to-use, portable and economical, the test is ideal for monitoring raw materials, as well as manufacturing and filling processes.

Benefits

- Small and easy to handle for on-the-spot analysis
- Bar-code calibration for reliable quantitative results in minutes
- Low analysis costs

For more details, please visit: www.merckmillipore.com/aaf





Reflectometry **Reflectoquant®**

General information	116
Are your vegetables healthy?	116
RQflex® 10	118
Is your diet drink really sugar free?	119
Test kits	120



Food & beverage workflow
> Page 30

Reflectometric measurements

Take your lab to the sample with the **Reflectoquant®** system. Compact and easy-to-use, the system allows you to monitor raw materials in all stages of your production processes, and obtain precise quantitative results – directly on-site.

Consisting of test strips, and reflectometers, this comprehensive program gives you all the tools you need for high quality, low cost analysis. It also offers numerous tests with a broad range of parameters, measuring ranges and applications for the widest spectrum of sample materials.



Are your vegetables healthy?

Food & beverage workflow
> Page 30



Easy, on-the-spot determination of nitrate content

The application

- Humans ingest nitrate mostly through vegetables (70%), but also drinking water (20%) and cured meats (10%).
- Nitrate itself is not harmful, but its metabolic products can be.
- The World Health Organization recommends a daily limit of 3.65 mg nitrate per kg bodyweight.

Our solution: Reflectoquant® Nitrate Test

The Reflectoquant® Nitrate Test is designed for rapid, accurate determination of nitrate content in a variety of foods, such as vegetables or infant meals, and drinking water. To further support your analysis, we offer application notes for over 15 sample materials.

Benefits

- Fast analysis with reliable results
- Compact size for on-the-spot analysis
- Many applications available
- Low analysis costs
- Environmentally friendly

easy
disposal

Reliable results
with bar-code
calibration

fast results

with $\pm 10\text{--}15\%$ accuracy



Further Reflectoquant® applications

Test vitamin C content in food

Vitamin C (ascorbic acid) is an essential characteristic of many foods. Its depletion should be monitored as it signifies a deterioration of food quality and taste.

See our Reflectoquant® Ascorbic Acid Test applications for over 15 sample materials.
www.merckmillipore.com/aaf

Monitor acrylamide formation

In fried or baked goods, like potato chips, the reaction between asparagine and reducing sugars (fructose, glucose, etc.) may produce acrylamide, which is considered toxic and carcinogenic. Consequently, maximum limits of reducing sugars in potatoes should not be exceeded.

See our application "Total sugar in potatoes" for Reflectoquant® Total Sugar Test.
www.merckmillipore.com/aaf

Reflectoquant®

Mobile accuracy with test strips

RQflex® 10 reflectometer


RQflex® 10 reflectometers are designed for fast determination of more than 30 parameters using Reflectoquant® test strips. The instruments can store up to five different methods and 50 measurement values.



RQflex® 10		Ord. No. 1.16970.0001
Scope of delivery	Includes test-strip adapter and recalibration set, double optical system (option for evaluation for two reaction zones), memory for five methods, memory slots for 50 results (with date, time, parameter, and result), batch-specific calibration function (bar-code technology), battery operation with 4 1.5-V batteries, detailed manual for reflectometer and tests	

RQflex® accessories | sample preparation | quality assurance

Product	Application	Ord. No.
Test strip adapter for RQflex® 10		1.16953.0001
Recalibration set for RQflex® 10		1.16954.0001
RQcheck check set for RQflex® 10		1.16957.0001
Polyvinylpolypyrrolidone Divergan® RS, 100 g	Decolorization	1.07302.0100
Sodium azide tablets, 5,000 tabs	Preserving milk samples	1.06687.0001
Potassium dichromate tablets, 5,000 tabs	Preserving milk samples	1.04858.0001

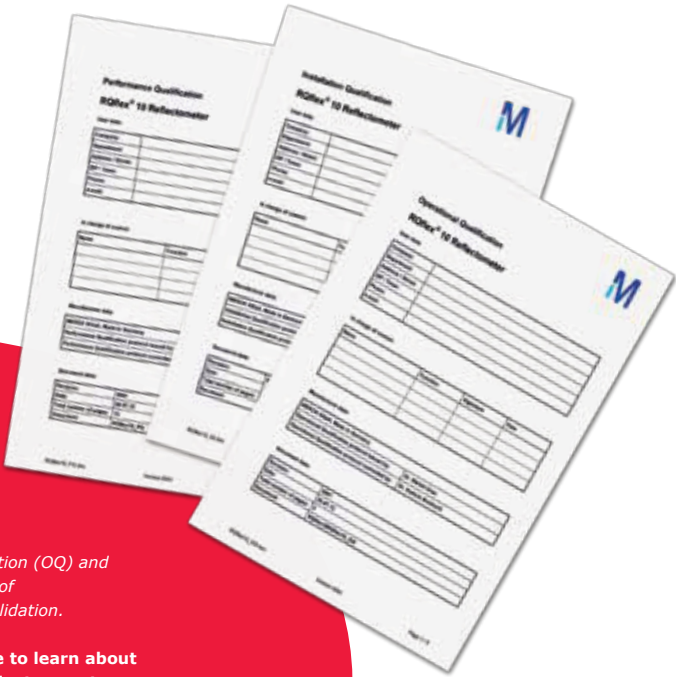

! IQ, OQ and PQ documents
Installation qualification (IQ), operational qualification (OQ) and performance qualification (PQ) are essential parts of quality assurance, achieved through equipment validation.

Please contact your local sales representative to learn about our validation services for all Reflectoquant® instruments.

! ANALYTICAL APPLICATION NOTES FINDER

Interested in more application examples?

Visit www.merckmillipore.com/aaf

> **Reflectometry**

Is your diet drink really sugar free?


If you use the same production line for diet and non-diet beverages, you need to be sure that your entire production system is free from sugar.

We offer a fast and easy solution: check your production line with RQflex® test strips for glucose and total sugar, and you'll have precise results within minutes.

Ord. No. 1.16720.0001 (glucose) and 1.16136.0001 (total sugar)



Food & beverage workflow
> Page 30

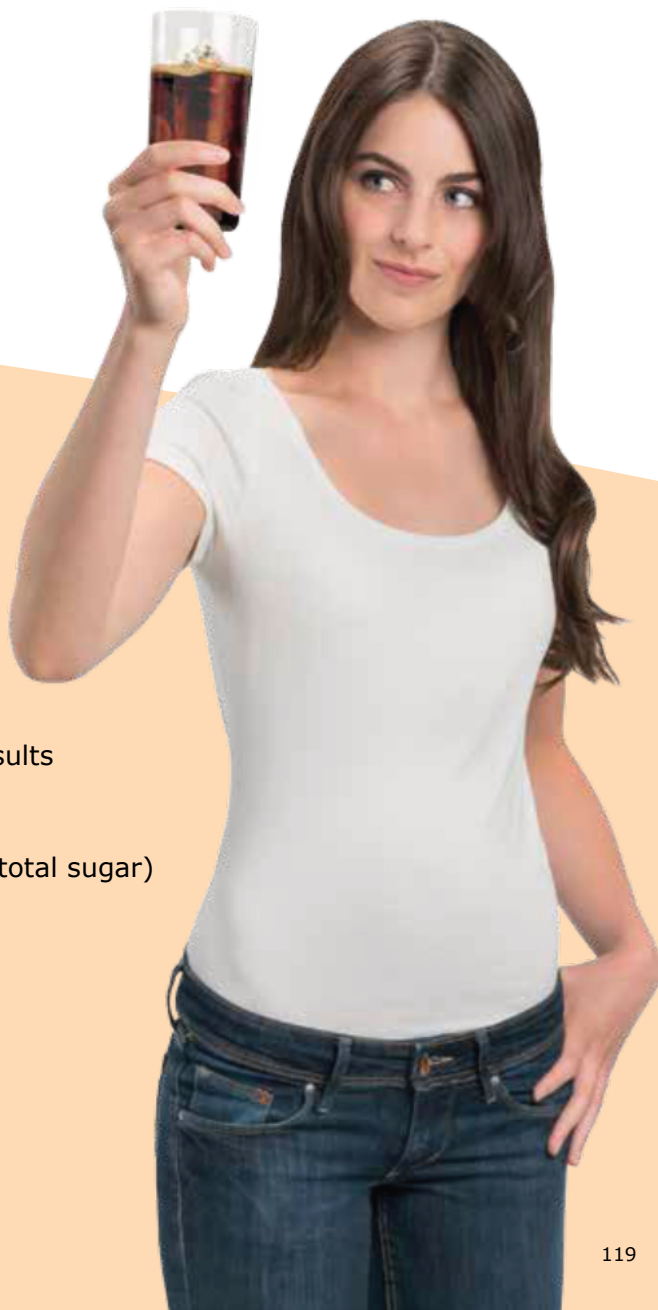

	Parameter	Graduation	No. of tests	Ord. No.	Method	Type
A	Ammonium Test	0.2 – 7.0 mg/L NH ₄	50	1.16892.0001	Indophenol blue	Reagent, incl.
	Ammonium Test	5.0 – 20.0 mg/L NH ₄	50	1.16899.0001	Indophenol blue	Reagent, incl.
	Ammonium Test	20 – 180 mg/L NH ₄	50	1.16977.0001	Nessler	Reagent, incl.
	Ascorbic Acid Test	25 – 450 mg/L ascorbic acid	50	1.16981.0001	Phosphormolybd. blue	
	Ascorbic Acid Test RQeasy®	25 – 450 mg/L ascorbic acid	50	1.17963.0001	Phosphormolybd. blue	
B	Blank Strip		50	1.16730.0001		
C	Calcium Test	2.5 – 45.0 mg/L Ca	50	1.16993.0001	Glyoxal-bis-(2-hydroxyanil)	Reagent, incl.
	Calcium Test	5 – 125 mg/L Ca	50	1.16125.0001	Phthalein complexone	
	Chlorine Test (free chlorine)	0.5 – 10.0 mg/L Cl ₂	50	1.16896.0001	Redox reaction	Reagent, incl.
F	Formaldehyde Test	1.0 – 45.0 mg/L HCHO	50	1.16989.0001	Triazole	Reagent, incl.
G	Glucose Test	1 – 100 mg/L glucose	50	1.16720.0001	Enzymatic reaction	
H	Hydroxymethylfurfural Test	1.0 – 60.0 mg/L HMF	50	1.17952.0001	Enzymatic reaction	
I	Iron Test	0.5 – 20.0 mg/L Fe(II)	50	1.16982.0001	Triazine	
	Iron Test	20 – 200 mg/L Fe(II)	50	1.16983.0001	2,2'-Bipyridine	
L	Lactic Acid Test	3.0 – 60.0 mg/L lactic acid	50	1.16127.0001	Enzymatic reaction	
M	Magnesium Test	5 – 100 mg/L Mg	50	1.16124.0001	Phthalein complexone	
	Malic Acid Test	5.0 – 60.0 mg/L malic acid	50	1.16128.0001	Enzymatic reaction	
	Nitrate Test	3 – 90 mg/L NO ₃	50	1.16995.0001	Modified Griess' reaction	
N	Nitrate Test	5 – 225 mg/L NO ₃	50	1.16971.0001	Modified Griess' reaction	
	Nitrate Test RQeasy®	5 – 250 mg/L NO ₃	50	1.17961.0001	Modified Griess' reaction	
	Nitrite Test	0.5 – 25.0 mg/L NO ₂	50	1.16973.0001	Griess' reaction	
	Nitrite Test	0.03 – 1.00 g/L NO ₂	50	1.16732.0001	Aromatic amine	
	Peracetic Acid Test	1.0 – 22.5 mg/L peracetic acid	50	1.16975.0001	Redox reaction	
P	Peracetic Acid Test	20.0 – 100 mg/L peracetic acid	50	1.17956.0001	Redox reaction	
	Peracetic Acid Test	75 – 400 mg/L peracetic acid	50	1.16976.0001	Redox reaction	
	Peroxide Test	0.2 – 20.0 mg/L H ₂ O ₂	50	1.16974.0001	Enzymatic reaction	
	Peroxide Test	20.0 – 100 mg/L H ₂ O ₂	50	1.17968.0001	Enzymatic reaction	
	Peroxide Test	100 – 1,000 mg/L H ₂ O ₂	50	1.16731.0001	Enzymatic reaction	
	pH Test	pH 1.0 – 5.0	50	1.16894.0001	Mixed indicator	
	pH Test	pH 4.0 – 9.0	50	1.16996.0001	Mixed indicator	
	pH Test for Cooling Lubricants	pH 7.0 – 10.0	50	1.16898.0001	Mixed indicator	
	Phosphate Test RQflex® plus	0.1 – 5.0 mg/L PO ₄	100	1.17942.0001	Phosphormolybd. blue	
	Phosphate Test	5 – 120 mg/L PO ₄	50	1.16978.0001	Phosphormolybd. blue	Reagent, incl.
	Potassium Test RQflex® plus	1.0 – 25.0 mg/L K	100	1.17945.0001	Kalignost®, turbidimetric	
	Potassium Test	0.25 – 1.20 g/L K	50	1.16992.0001	Dipicrylamine	Reagent, incl.
	Sucrose Test	0.25 – 2.50 g/L	50	1.16141.0001	Enzymatic reaction	Reagent, incl.
S	Sulfite Test	10 – 200 mg/L SO ₃	50	1.16987.0001	Nitroprusside / Zn-hexacyanoferrate	
T	Total Hardness Test	0.1 – 30.0 °d	50	1.16997.0001	Phthalein complexone	
	Total Sugar Test (glucose and fructose)	65 – 650 mg/L total sugar	50	1.16136.0001	Enzymatic reaction	Reagent, incl.
U	Urea Test in Milk Application	0.2 – 7.0 mg/L NH ₄	50	1.16892.0001	Indophenol blue	Reagent, incl.

Watch our videos and learn how to use our reflectometry instruments and test kits



[www.merckmillipore.com/
video_asp_wfa_ascorbic_acid](https://www.merckmillipore.com/video_asp_wfa_ascorbic_acid)



[www.merckmillipore.com/
video_asp_wfa_reflectoquant_
maintenance](https://www.merckmillipore.com/video_asp_wfa_reflectoquant_maintenance)

	Beer processing	Food testing	Juices	Milk products	Mineral water	Soft drinks	Aquaculture	Boiler water, cooling water	Drinking water	Groundwater, surface water	Industrial water	Process water	Seawater	Swimming pools	Wastewater	Agriculture	Disinfection control	Electroplating	Parameter
	Food and beverages						Water (Analytics)							Others					
							■		■	■			■		■	■			Ammonium Test
							■		■	■			■		■	■			Ammonium Test
															■	■			Ammonium Test
	■	■	■	■		■													Ascorbic Acid Test
	■	■	■	■		■													Ascorbic Acid Test RQeasy®
	■	■	■	■		■													Blank Strip
	■	■	■	■	■	■		■	■	■	■				■				Calcium Test
	■	■	■	■	■	■		■	■	■									Calcium Test
									■						■		■		Chlorine Test
															■		■		Formaldehyde Test
	■	■	■	■		■													Glucose Test
		■	■							■	■		■		■				Hydroxymethylfurfural Test
		■	■		■					■	■				■			■	Iron Test
		■	■		■					■	■				■			■	Iron Test
	■	■	■	■		■													Lactic Acid Test
		■			■			■	■	■						■			Magnesium Test
		■	■			■													Malic Acid Test
		■	■		■	■	■		■	■	■		■		■	■			Nitrate Test
		■	■		■	■	■		■	■	■		■		■	■			Nitrate Test
		■	■		■		■		■	■	■		■		■	■			Nitrate Test RQeasy®
		■					■			■			■		■				Nitrite Test
								■											Nitrite Test
																	■		Peracetic Acid Test
																	■		Peracetic Acid Test
																	■		Peracetic Acid Test
														■			■		Peroxide Test
																	■		Peroxide Test
																	■		Peroxide Test
		■	■	■	■	■			■	■	■	■		■	■	■			pH Test
		■	■		■	■	■		■	■	■	■		■	■	■			pH Test
		■					■		■	■			■		■	■		■	pH Test for Cooling Lubricants
		■							■	■					■	■			Phosphate Test RQflex® plus
		■													■	■			Phosphate Test
			■						■	■						■			Potassium Test RQflex® plus
	■		■		■	■			■		■				■	■			Potassium Test
	■	■	■	■		■													Sucrose Test
		■						■							■				Sulfite Test
					■			■	■	■									Total Hardness Test
	■	■	■			■													Total Sugar Test (glucose and fructose)
				■															Urea Test in Milk Application

AIM FOR BRILLIANCE

Is your water
of the highest
quality?

Detect very low concentrations of impurities in water

The application

- Drinking water, groundwater, freshwater, mineral water and process water should be regularly tested for a variety of parameters.
- Analysis often requires high measurement sensitivities down to the ppb range.

Our solution: MColortest™ with color-card comparator

The MColortest™ system is designed for highly sensitive, fast analysis of any water sample. It includes a color-card comparator, which allows you to compare the reaction color of the sample with a high-quality color scale for accurate evaluation.

Benefits

- Unique brilliance and fine color graduation for precise analysis
- Easy-to-use visual tests with fast results
- Very low (ppb range) to medium concentrations can be tested
- Excellent measurement sensitivity

For more details, please visit: www.merckmillipore.com/aaf





Colorimetric and titrimetric test kits

MColortest™

General information	124
Is the water's ammonium level safe for aquatic life?	125
Visual rapid tests	126
Product list	128
Compact laboratory	137



Cooling & boiler water workflow
> Page 20



Drinking water workflow
> Page 24



Bottled water workflow
> Page 26



Colorimetric and titrimetric test kits

MColortest™ test kits give you exceptional results with brilliant color cards for easy, precise comparison. No special training is required – simply follow our illustrated instructions. Despite their simplicity, they offer unparalleled reliability. All test kits are thoroughly checked using certified standard solutions, which can be traced directly to primary reference materials from NIST and PTB. Thanks to their excellent stability, the kits can be stored for up to three years at 15-25°C.



The MColortest™ system includes colorimetric and titrimetric tests (evaluation using color cards or test vessels, respectively). For more information, please see page 126.

Economical
refill packs

Easy, fast,
direct read-out of color cards

Maximum
reliability
with numerous parameters

Is the water's ammonium level safe for aquatic life?


Sensitive measurement of ammonium in fresh- and seawater

The application

- Ammonium is a common water pollutant and can be toxic to aquatic life.
- Measuring the ammonium concentration of water is required by many international authorities, and maximum limits may not be exceeded.

Our solution: MColortest™ Ammonium Test

We offer special test kits for fast, reliable measurement of ammonium ions and unionized ammonium in fresh- or seawater. The kits are designed for use with the MColortest™ system, offering sensitive measurements in the range of 0.5 to 10 mg/L NH_4 .

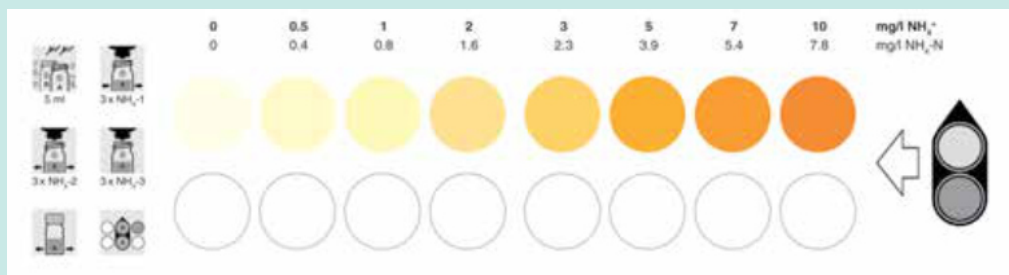

Benefits

- Easy to use with illustrated instructions
- Color card included in test kit for precise comparison
- Fast reaction times with results in 10 minutes
- Waste disposal advice available

For more applications, please visit: www.merckmillipore.com/aaf

High to medium concentrations, especially for turbid solutions MColortest™ with color-disk comparator

These tests evaluate the color reaction based on the transmitted light method. So even turbid and lightly colored water samples can be analyzed without further preparation.

Ten-stage color disk is made of very durable, lightfast plastic, thus suitable for industrial areas and wet environments. Almost all test vessels are break-proof for safer handling.

Application areas:

- Wastewater
- Industrial water
- Groundwater
- Bottled water
- Boiler water
- Swimming pool water
- Industrial applications

*The MColortest™ system:
All reagents and the
color-disk comparator are
contained in the kit.*



Medium concentrations MColortest™ titrimetric and colorimetric methods

Titrimetric test: Sample is titrated until its color changes. Number of drops consumed to the turning point are counted, or the scale value is read from a pipette to determine the concentration of the tested parameter.

Colorimetric test: Reagents are added to the sample, resulting in a color reaction. Concentration is determined by allocating the color to a value on a reference scale.



Application areas:

- Aquaculture for freshwater and seawater
- Surface water
- Swimming pool water
- School lessons

Very low to medium concentrations MColortest™ with color-card comparator


The comparator's greater layer thickness and special construction ensure high measurement sensitivity, even at very low concentrations (ppb range).

The sample's reaction color is compared with the blank sample tinted by the color cards to determine concentration. The brilliant print and fine color graduation enable precise analyses.

Application areas:

- Drinking water
- Bottled water
- Boiler water
- Cooling water
- Industrial applications

*MColortest™ and the
color-card comparator offer
unparalleled reliability!*

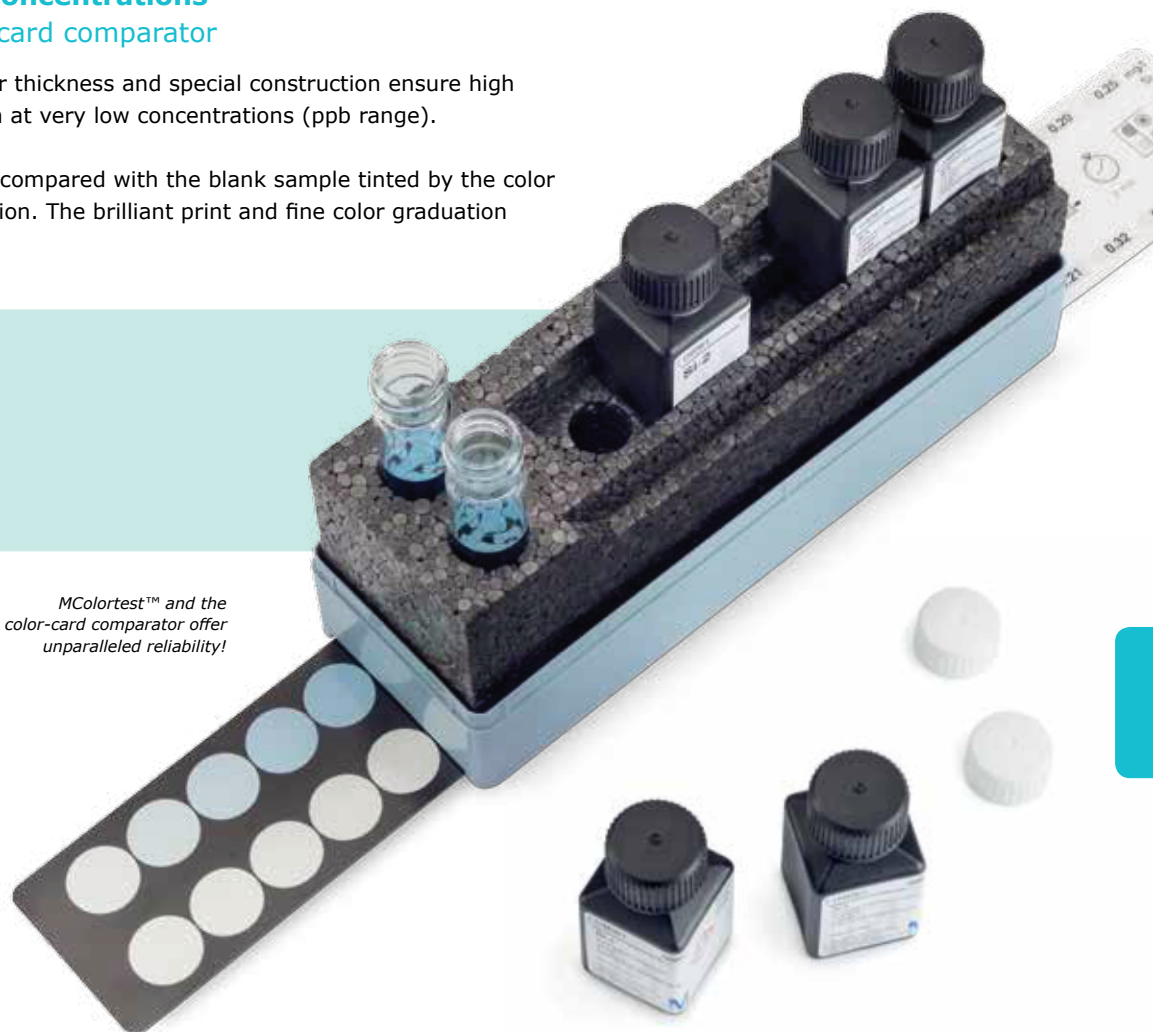

! Practical refill packs

You can effectively reduce your costs per analysis by using the economical refill packs we offer for many of our test kits.

! Waste disposal advice

Get detailed information about disposal of MColortest™ kits on:
www.disposal-test-kits.com

	Parameter	Graduation	No. of tests	Ord. No.	Ord. No. Refill pack	Method	Type
A	Alkalinity Test	0.1 mmol/L	200 at 8.5 mmol/L	1.11109.0001		Acidimetric	Titration with pipette
	Aluminium Test	0.07–0.12–0.20–0.35–0.50–0.65–0.80 mg/L Al	185	1.14413.0001	1.18452.0002	Chromazurol S	Color-card comparator
	Aluminium Test	0.10–0.20–0.35–0.50–0.75–1–2–3–6 mg/L Al	150	1.18386.0001	1.18452.0002	Chromazurol S	Disk comparator
	Ammonium Test	0.025–0.050–0.075–0.10–0.15–0.20–0.25–0.30–0.40 mg/L NH ₄	70	1.14428.0002		Indophenol blue	Color-card comparator
	Ammonium Test	0.05–0.10–0.15–0.2–0.3–0.4–0.5–0.6–0.8 mg/L NH ₄	100	1.14400.0001		Neßler	Color-card comparator
	Ammonium Test	0.2–0.4–0.6–1–2–3–5 mg/L NH ₄	50	1.08024.0001		Indophenol blue	Sliding comparator
	Ammonium Test	0.2–0.5–0.8–1.2–1.6–2–3–5–8 mg/L NH ₄	200	1.14423.0002	1.18455.0002	Indophenol blue	Color-card comparator
	Ammonium Test	0.2–0.5–0.8–1.3–2.0–3.0–4.5–6.0–8.0 mg/L NH ₄	200	1.14750.0002	1.18455.0002	Indophenol blue	Disk comparator
	Ammonium Test	0.5–1–3–5–10 mg/L NH ₄	150	1.11117.0001		Neßler	Color-card comparator
	Ammonium Test in freshwater and seawater	0.5–1–3–5–10 mg/L NH ₄	50	1.14657.0001		Indophenol blue	Color card
C	Calcium Test	2 mg/L Ca	200 at 170 mg/L Ca	1.11110.0001		Titriplex® III	Titration with pipette
	Carbon Dioxide Test	1.25 mg/L CO ₂ 2.5 mg/L CO ₂ 5 mg/L CO ₂	100 at 30 mg/L 100 at 60 mg/L 100 at 120 mg/L	1.17179.0001		Phenolphthalein	Titration with dropping bottle
	Carbonate Hardness Test/ Acid cap. to pH 4.3 (ANC)	0.25 °e and 0.1 mmol/L	300 at 12.5 °e	1.08048.0001		Acidimetric	Titration with pipette
	Carbonate Hardness Test/ Acid cap. to pH 4.3 (ANC)	1.25 °e	100 at 12.5 °e	1.11103.0001		Acidimetric	Titration with dropping bottle
	Carbonate Hardness Test in freshwater and seawater	1.25 °e	50 at 1.25 °e	1.14653.0001		Acidimetric	Titration with dropping bottle
	Chloride Test	2 mg/L Cl	200 at 170 mg/L Cl	1.11106.0001		Mercury(II)-nitrate	Titration with pipette
	Chloride Test	3–6–10–18–30–60–100–180–300 mg/L Cl	200	1.14753.0001	1.18322.0002	Mercury(II)-thiocyanate	Disk comparator
	Chloride Test	5–10–20–40–75–150–300 mg/L Cl	400	1.14401.0001	1.18322.0002	Mercury(II)-thiocyanate	Color-card comparator
	Chloride Test	25 mg/L Cl	100 at 150 mg/L Cl	1.11132.0001		Mercury(II)-nitrate	Titration with dropping bottle
	Chlorine Test (free chlorine)	0.01–0.025–0.045–0.06–0.08–0.1–0.15–0.2–0.3 mg/L Cl ₂	400 free chlorine	1.14434.0001	1.14977.0002	DPD	Color-card comparator
	Chlorine Test (free chlorine) in freshwater and seawater	0.10–0.25–0.5–1.0–2.0 mg/L Cl ₂	100 free chlorine	1.14670.0001		TMB	Color card
	Chlorine Test (free chlorine)	0.1–0.2–0.3–0.4–0.6–0.8–1.0–1.5–2.0 mg/L Cl ₂	600 free chlorine	1.14978.0001	1.14979.0002	DPD Liquid	Disk comparator
	Chlorine Test (free and total chlorine)	0.1–0.2–0.3–0.4–0.6–0.8–1.0–1.5–2.0 mg/L Cl ₂	400 free chlorine + 400 total chlorine	1.14801.0001	1.14803.0002	DPD Liquid	Disk comparator
	Chlorine Test (free chlorine)	0.25–0.50–0.75–1–2–4–8–10–15 mg/L Cl ₂	1,000 free chlorine	1.14976.0001	1.14977.0002	DPD	Disk comparator

	Beer processing	Food testing	Juices	Milk products	Mineral water	Soft drinks	Aquaculture	Boiler water, cooling water	Drinking water	Groundwater, surface water	Industrial water	Process water	Seawater	Swimming pools	Wastewater	Agriculture	Disinfection control	Electroplating	Parameter
	Food and beverages						Water (Analytics)								Others				
					■		■	■	■	■	■	■	■	■					Alkalinity Test
	■				■		■	■	■	■	■	■	■	■				■	Aluminium Test
	■				■		■	■	■	■	■	■	■	■				■	Aluminium Test
		■			■		■	■	■	■				■	■	■			Ammonium Test
							■	■	■	■				■	■	■			Ammonium Test
		■			■		■	■	■	■	■			■	■	■			Ammonium Test
		■			■		■	■	■	■	■			■	■	■		■	Ammonium Test
		■			■		■	■	■	■	■			■	■	■		■	Ammonium Test
							■	■	■	■	■	■	■	■					Ammonium Test
							■		■	■			■	■		■			Ammonium Test in freshwater and seawater
					■		■	■	■	■					■				Calcium Test
								■	■	■	■		■		■				Carbon Dioxide Test
					■		■	■	■	■	■	■							Carbonate Hardness Test / Acid cap. to pH 4.3 (ANC)
					■		■	■	■	■	■	■							Carbonate Hardness Test / Acid cap. to pH 4.3 (ANC)
					■		■	■	■	■	■	■							Carbonate Hardness Test in freshwater and seawater
		■			■		■	■	■	■	■	■	■	■	■	■			Chloride Test
		■			■		■	■	■	■	■	■	■	■	■	■			Chloride Test
		■			■		■	■	■	■	■	■	■	■	■	■			Chloride Test
		■			■		■	■	■	■	■	■	■	■	■	■			Chloride Test
					■		■		■						■		■	■	Chlorine Test (free chlorine)
					■		■		■	■		■			■				Chlorine Test (free chlorine) in freshwater and seawater
					■		■		■	■					■		■	■	Chlorine Test (free chlorine)
					■		■		■	■				■	■		■	■	Chlorine Test (free and total chlorine)
					■		■		■	■					■		■	■	Chlorine Test (free chlorine)

	Parameter	Graduation	No. of tests	Ord. No.	Ord. No. Refill pack	Method	Type
C	Chlorine Test (free and total chlorine)	0.25–0.50–0.75–1–2– 4–7–10–15 mg/L Cl ₂	400 free chlorine + 400 total chlorine	1.14826.0001	1.18326.0002	DPD	Disk comparator
	Chlorine- and pH Test (free chlorine)	0.10–0.20–0.30–0.60–1.0–1.5 mg/L Cl ₂ / pH 6.5–6.8–7.0–7.2–7.4–7.6–7.9	150 (chlorine) 150 (pH)	1.11160.0001		DPD Phenol red	Sliding comparator
	Chlorine- and pH Test (free and total chlorine)	0.1–0.3–0.6–1.0–1.5 mg/L Cl ₂ pH 6.8–7.1–7.4–7.6–7.8	200 (chlorine) 200 (pH)	1.11174.0001	1.11157.0001 1.11143.0001	DPD Phenol red	Color-matching vessel
	Chlorine Dioxide Test	0.020–0.050–0.075–0.10–0.15– 0.20–0.30–0.40–0.55 mg/L ClO ₂	300	1.18754.0001	1.18757.0002	DPD	Color-card comparator
	Chlorine Dioxide Test	0.5–0.9–1.4–1.9–3.8–7.5– 13–19–28 mg/L ClO ₂	300	1.18756.0001	1.18757.0002	DPD	Disk comparator
	Chromate Test	0.011–0.022–0.045–0.07–0.09– 0.11–0.13–0.18–0.22 mg/L CrO ₄	150	1.14402.0001	1.18456.0002	Diphenyl- carbazide	Color-card comparator
	Chromate Test	0.22–0.45–0.67–1.0–1.3–1.8– 2.2–2.9–3.6 mg/L CrO ₄	300	1.14441.0001	1.18456.0002	Diphenyl- carbazide	Color-card comparator
	Chromate Test	0.22–0.45–0.8–1.3–2.2–4.0– 6.7–13–22 mg/L CrO ₄	300	1.14756.0001	1.18456.0002	Diphenyl- carbazide	Disk comparator
	Color Test	5–10–20–30–40–50– 70–100–150 CU (Hazen)	no limit	1.14421.0001		Hazen	Color-card comparator
	Copper Test	0.05–0.08–0.12–0.16–0.2– 0.25–0.3–0.4–0.5 mg/L Cu	125	1.14414.0001	1.18459.0002	Cuprizone	Color-card comparator
	Copper Test in freshwater and seawater	0.15–0.3–0.45–0.6–0.8– 1.2–1.6 mg/L Cu	50	1.14651.0001		Cuprizone	Color card
	Copper Test	0.3–0.6–1.0–1.5–2.0–2.5– 3–5 mg/L Cu	125	1.14418.0001	1.18459.0002	Cuprizone	Color-card comparator
	Copper Test	0.3–0.6–1.0–1.5–2–3– 5–7–10 mg/L Cu	125	1.14765.0001	1.18459.0002	Cuprizone	Disk comparator
	Cyanide Test	0.002–0.004–0.007–0.010–0.013– 0.016–0.020–0.025–0.030 mg/L CN	65	1.14417.0001	1.18457.0002	König reaction	Color-card comparator
	Cyanide Test	0.03–0.06–0.10–0.15–0.2– 0.3–0.4–0.5–0.7 mg/L CN	200	1.14429.0001	1.18457.0002	König reaction	Color-card comparator
	Cyanide Test	0.03–0.07–0.13–0.2–0.3– 0.5–1–2–5 mg/L CN	200	1.14798.0001	1.18457.0002	König reaction	Disk comparator
F	Fluoride Test	0.15–0.3–0.5–0.8 mg/L F	100	1.18771.0001		Alizarin complexone	Color card
	Formaldehyde Test	0.10–0.25–0.4–0.6–0.8– 1.0–1.5 mg/L HCHO	100	1.08028.0001		Triazole derivative	Sliding comparator
H	Hydrazine Test	0.10–0.25–0.5–1.0 mg/L N ₂ H ₂	100	1.08017.0001	necessary 1.08018.0001	Dimethylamino- benzaldehyde	Color-matching vessel
I	Iron Test	0.01–0.02–0.03–0.04–0.06– 0.08–0.10–0.15–0.20 mg/L Fe	300	1.14403.0001	1.18458.0002	Triazine	Color-card comparator
	Iron Test in freshwater and seawater	0.05–0.1–0.2–0.4– 0.6–0.8–1.0 mg/L Fe	50	1.14660.0001		Triazine	Color card
	Iron Test	0.1–0.2–0.5–0.8–1.2– 2–3–5 mg/L Fe	500	1.14759.0001	1.18458.0002	Triazine	Disk comparator
	Iron Test	0.1–0.3–0.5–1.0–2.5– 5.0–7.5–12.5–25–50 mg/L Fe	200	1.11136.0001	1.08023.0001	2,2'-Bipyridine	Color-matching vessel
	Iron Test	0.2–0.4–0.6–0.8–1.0–1.3– 1.6–2.0–2.5 mg/L Fe	500	1.14438.0001	1.18458.0002	Triazine	Color-card comparator

	Beer processing	Food testing	Juices	Milk products	Mineral water	Soft drinks	Aquaculture	Boiler water, cooling water	Drinking water	Groundwater, surface water	Industrial water	Process water	Seawater	Swimming pools	Wastewater	Agriculture	Disinfection control	Electroplating	Parameter
	Food and beverages						Water (Analytics)								Others				
								■						■	■		■		Chlorine Test (free and total chlorine)
														■					Chlorine- and pH Test (free chlorine)
														■					Chlorine- and pH Test (free and total chlorine)
							■	■									■		Chlorine Dioxide Test
							■	■			■				■		■		Chlorine Dioxide Test
								■	■	■		■			■			■	Chromate Test
								■	■	■		■			■			■	Chromate Test
								■	■	■		■			■			■	Chromate Test
	■		■			■		■	■		■				■			■	Color Test
	■	■	■			■		■	■			■	■	■				■	Copper Test
							■	■	■	■		■	■	■					Copper Test in freshwater and seawater
		■						■	■	■		■	■	■				■	Copper Test
		■						■	■	■		■	■	■				■	Copper Test
		■			■		■		■	■	■				■			■	Cyanide Test
					■		■		■	■	■				■			■	Cyanide Test
					■		■		■	■	■				■			■	Cyanide Test
					■			■	■										Fluoride Test
		■									■						■	■	Formaldehyde Test
							■												Hydrazine Test
		■			■		■	■	■	■	■		■		■				Iron Test
					■		■	■	■	■		■			■				Iron Test in freshwater and seawater
					■		■	■	■	■		■			■				Iron Test
		■			■		■	■	■	■					■				Iron Test
		■			■		■	■	■	■		■			■				Iron Test

	Parameter	Graduation	No. of tests	Ord. No.	Ord. No. Refill pack	Method	Type
I	Iron Test	0.25–0.5–1.0–2.0–3.0–5.0– 7.5–10–15 mg/L Fe	300	1.14404.0001		1,10-phenanthroline	Color-card comparator
M	Magnesium Test	100–200–300–500– 1,000–1,500 mg/L Mg	50	1.11131.0001		Xylidyl blue	Color card
	Manganese Test	0.03–0.06–0.10–0.15–0.20– 0.25–0.3–0.4–0.5 mg/L Mn	120	1.14406.0001	1.18460.0002	Oxime	Color-card comparator
	Manganese Test	0.3–0.7–1.3–2–3–4– 5–7–10 mg/L Mn	120	1.14768.0001	1.18460.0002	Oxime	Disk comparator
N	Nickel Test	0.02–0.04–0.07–0.10–0.15– 0.2–0.3–0.4–0.5 mg/L Ni	125	1.14420.0001	1.18461.0002	Dimethyl-glyoxime	Color-card comparator
	Nickel Test	0.5–1.0–1.5–2–3–4–6– 8–10 mg/L Ni	500	1.14783.0001	1.18461.0002	Dimethyl-glyoxime	Disk comparator
	Nitrate Test	5–10–20–30–40–50–60– 70–90 mg/L NO ₃	90	1.18387.0001	1.18462.0002	Nitrospectral / sulfuric acid	Disk comparator
	Nitrate Test	10–25–50–75–100–125– 150 mg/L NO ₃	200	1.11170.0001		Sulfanilic acid	Sliding comparator
	Nitrate Test in freshwater	10–25–50–75–100–125– 150 mg/L NO ₃	100	1.11169.0001		Sulfanilic acid	Color card
	Nitrite Test	0.005–0.012–0.02–0.03–0.04– 0.05–0.06–0.08–0.10 mg/L NO ₂	110	1.14408.0001	1.18463.0002	Griess' reaction	Color-card comparator
	Nitrite Test in freshwater and seawater	0.05–0.15–0.25–0.50–1.0 mg/L NO ₂	100	1.14658.0001		Griess' reaction	Color card
	Nitrite Test	0.025–0.05–0.075–0.1–0.15– 0.2–0.3–0.5 mg/L NO ₂	200	1.08025.0001		Griess' reaction	Sliding comparator
	Nitrite Test	0.1–0.2–0.3–0.4–0.6–0.8– 1.0–1.3–2.0 mg/L NO ₂	400	1.14424.0001	1.18463.0002	Griess' reaction	Color-card comparator
	Nitrite Test	0.1–0.2–0.4–0.6–1.0–1.8– 3.0–6.0–10 mg/L NO ₂	400	1.14774.0001	1.18463.0002	Griess' reaction	Disk comparator
O	Oxygen Test	0.1 mg/L O ₂	100 at 8.5 mg/L O ₂	1.11107.0001	1.11152.0001 1.14663.0001	modified Winkler method	Titration with pipette
	Oxygen Test in freshwater and seawater	1–3–5–7–9–12 mg/L O ₂	50	1.14662.0001	necessary: 1.14663.0001	modified Winkler method	Color card
	Ozone Test	0.007–0.017–0.030–0.040–0.055– 0.070–0.10–0.14–0.20 mg/L O ₃	300	1.18755.0001	1.18759.0002	DPD	Color-card comparator
	Ozone Test	0.15–0.35–0.5–0.7–1.4– 2.7–5.0–7.0–10 mg/L O ₃	300	1.18758.0001	1.18759.0002	DPD	Disk comparator
P	pH Universal indicator, liquid	pH 4.0–4.5–5.0–5.5–6.0–6.5– 7.0–7.5–8.0–8.5–9.0–9.5–10.0	100 mL	1.09175.0100		Mixed indicator	Color card
	pH Universal indicator, liquid	pH 4.0–4.5–5.0–5.5–6.0–6.5– 7.0–7.5–8.0–8.5–9.0–9.5–10.0	1 L	1.09175.1000		Mixed indicator	Color card
	pH Indicator liquid	pH 9.0–10.0–11.0–12.0–13.0	100 mL	1.09176.0100		Mixed indicator	Color card
	pH Test	pH 4.5–5.0–5.5–6.0–6.5–7.0– 7.5–8.0–8.5–9.0	400	1.08027.0001		Mixed indicator	Sliding comparator
	pH Test	pH 4.5–5.0–5.5–6.0–6.5– 7.0–7.5–8.0–8.5–9.0	100	1.08038.0001	1.08043.0001	Mixed indicator	Color-matching vessel
	pH Test in freshwater and seawater	pH 5.0–5.3–5.6–6.0–6.3–6.6– 7.0–7.3–7.6–8.0–8.3–8.6–9.0	200	1.18773.0001		Mixed indicator (fresh-/seawater)	Color-card comparator

	Beer processing	Food testing	Juices	Milk products	Mineral water	Soft drinks	Aquaculture	Boiler water, cooling water	Drinking water	Groundwater, surface water	Industrial water	Process water	Seawater	Swimming pools	Wastewater	Agriculture	Disinfection control	Electroplating	Parameter
	Food and beverages						Water (Analytics)								Others				
		■			■		■	■	■	■	■		■		■				Iron Test
									■	■									Magnesium Test
					■			■	■	■			■		■	■		■	Manganese Test
					■			■	■	■			■		■	■		■	Manganese Test
									■	■	■				■			■	Nickel Test
									■	■	■				■			■	Nickel Test
	■	■		■	■		■		■	■	■			■	■	■			Nitrate Test
		■					■		■	■				■	■	■			Nitrate Test
		■					■		■	■	■			■	■				Nitrate Test in freshwater
		■			■		■	■	■	■			■		■	■		■	Nitrite Test
				■			■	■	■	■	■		■		■				Nitrite Test in freshwater and seawater
		■			■		■	■	■	■			■		■	■		■	Nitrite Test
		■			■		■	■	■	■			■		■	■		■	Nitrite Test
	■			■	■	■	■	■	■	■			■		■				Oxygen Test
							■		■	■			■		■				Oxygen Test in freshwater and seawater
									■			■		■	■		■		Ozone Test
									■			■		■	■		■		Ozone Test
	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	pH Universal indicator, liquid
	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	pH Universal indicator, liquid
														■				■	pH Indicator liquid
	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	■	pH Test
							■	■	■	■	■								pH Test
							■		■	■			■						pH Test in freshwater and seawater

	Parameter	Graduation	No. of tests	Ord. No.	Ord. No. Refill pack	Method	Type
P	pH Test in swimming pool	pH 6.5–6.8–7.1–7.4–7.6–7.8–8.2	200	1.14669.0001		Phenol red	Color card
	Phosphate Test	0.046–0.092–0.14–0.18–0.25–0.34–0.43 mg/L PO ₄	200	1.18394.0001	1.18465.0002	Phosphomolybdenum blue	Color-card comparator
	Phosphate Test in freshwater and seawater	0.25–0.50–0.75–1.0–1.5–2.0–3.0 mg/L PO ₄	100	1.14661.0001		Phosphomolybdenum blue	Color card
	Phosphate Test	0.6–1.2–1.8–2.5–3.1–4.6–6.1–7.7–9.2 mg/L PO ₄	200	1.14846.0001	1.18465.0002	Phosphomolybdenum blue	Disk comparator
	Phosphate Test	1.3–3.3–6.7–10–13 mg/L PO ₄	200	1.11138.0001	1.08046.0001	Phosphomolybdenum blue	Color-matching vessel
	Phosphate Test	3.1–6.1–11–18–31–61–123 mg/L PO ₄	190	1.14449.0001	1.18466.0002	Vanadium molybdate	Color-card comparator
	Phosphate Test	4.6–9.2–18–28–37–49–61–123–307 mg/L PO ₄	300	1.18388.0001	1.18466.0002	Vanadium molybdate	Disk comparator
R	Residual Hardness Test	0.05–0.10–0.19 °e	400	1.11142.0001		Mixed indicator	Color card
S	Silicate (Silicic Acid) Test	0.021–0.043–0.086–0.13–0.17–0.21–0.32–0.43–0.53 mg/L SiO ₂	150	1.14410.0001	1.18323.0002	Silico-molybdenum blue	Color-card comparator
	Silicate (Silicic Acid) Test	0.64–1.3–2.1–3.2–4.3–6.4–11–15–21 mg/L SiO ₂	150	1.14792.0001	1.18323.0002	Silico-molybdenum blue	Disk comparator
	Sulfate Test	25–50–75–100–130–160–190–240–300 mg/L SO ₄	75	1.18389.0001	1.18467.0002	Tannic acid	Disk comparator
	Sulfate Test	25–50–80–110–140–200–300 mg/L SO ₄	90	1.14411.0001	1.18467.0002	Tannic acid	Color-card comparator
	Sulfide Test	0.02–0.04–0.06–0.08–0.10–0.13–0.16–0.20–0.25 mg/L S	100	1.14416.0001	1.18468.0002	Dimethyl-p-phenyldiamine	Color-card comparator
	Sulfide Test	0.1–0.3–0.5–0.7–1–2–3–4–5 mg/L S	200	1.14777.0001	1.18468.0002	Dimethyl-p-phenyldiamine	Disk comparator
	Sulfite Test	0.5 mg/L Na ₂ SO ₃ (0.32 mg/L SO ₃)	200 at 40 mg/L Na ₂ SO ₃	1.11148.0001		Iodate / Starch	Titration with pipette
T	Total Hardness Test	0.13 °e and 1 mg/L CaCO ₃	300 at 3.8 °e	1.08047.0001	1.08040.0001	Titriplex® III	Titration with pipette
	Total Hardness Test	0.25 °e and 10 mg/L CaCO ₃	300 at 12.5 °e	1.08039.0001	1.08033.0001 1.11122.0001 1.08203.0001	Titriplex® III	Titration with pipette
	Total Hardness Test	1.25 °e	100 at 12.5 °e	1.11104.0001		Titriplex® III	Titration with dropping bottle
	Total Hardness Test	20 mg/L CaCO ₃	200 at 200 mg/L	1.08312.0001		Titriplex® III	Titration with dropping bottle
	Total Hardness Test in freshwater	1.25 °e	50 at 1.25 °e	1.14652.0001		Titriplex® III	Titration with dropping bottle
U	Urea Test for swimming pools	0.3–0.6–1.0–1.5–2–3–4–5–8 mg/L (NH ₂) ₂ CO	100	1.14843.0001	1.14845.0002	Indophenol blue	Disk comparator
Z	Zinc Test	0.1–0.2–0.3–0.4–0.5–0.7–1–2–5 mg/L Zn	120	1.14780.0001	1.14782.0002	Thiocyanate / Brilliant green	Disk comparator
	Zinc Test	0.1–0.2–0.3–0.4–0.5–0.7–1–2–5 mg/L Zn	120	1.14412.0001	1.14782.0002	Thiocyanate / Brilliant green	Color-card comparator

	Beer processing	Food testing	Juices	Milk products	Mineral water	Soft drinks	Aquaculture	Boiler water, cooling water	Drinking water	Groundwater, surface water	Industrial water	Process water	Seawater	Swimming pools	Wastewater	Agriculture	Disinfection control	Electroplating	Parameter
	Food and beverages						Water (Analytics)								Others				
														■					pH Test in swimming pool
		■							■	■			■		■	■		■	Phosphate Test
							■	■	■	■	■	■		■					Phosphate Test in freshwater and seawater
		■			■		■		■	■	■	■	■		■	■		■	Phosphate Test
		■			■		■	■	■	■	■	■			■	■		■	Phosphate Test
					■		■	■	■	■	■	■			■	■		■	Phosphate Test
					■		■	■	■	■	■	■			■	■		■	Phosphate Test
								■											Residual Hardness Test
					■			■	■	■	■	■	■		■				Silicate (Silicic Acid) Test
					■			■	■	■	■	■	■		■				Silicate (Silicic Acid)Test
					■				■	■					■				Sulfate Test
					■				■	■					■				Sulfate Test
					■		■		■	■					■	■			Sulfide Test
					■		■		■	■					■	■			Sulfide Test
	■	■	■	■	■	■		■	■	■					■				Sulfite Test
					■		■	■	■	■			■	■					Total Hardness Test
					■		■	■	■	■			■	■					Total Hardness Test
					■		■	■	■	■			■	■					Total Hardness Test
							■		■	■	■				■				Total Hardness Test in freshwater
													■	■					Urea Test
	■		■		■	■		■	■	■	■				■			■	Zinc Test
	■		■		■	■		■	■	■	■				■			■	Zinc Test

Is it time for an oil change?

We offer rapid colorimetric methods for determining the freshness of frying oils and fats. With our easy-to-use tests, you'll always know whether your oil is still good or if you need to replace it.



Deep-frying fats tests

Parameter	Graduation	No. of test	Ord. No.	Ord. No. Refill pack	Method
Free fatty acids	0.5–1.0–2.0–3.0 mg/g KOH	100	1.17046.0001		pH indicator
Oxifrit-Test®	fresh – change advisable – gone off	60 (Refill pack 30)	1.10653.0001	1.10654.0001	Colorimetric, acc. to the principle of determination of oxidized fatty acids (OFAs)

Accessories for MColortest™ and MQuant™

Product	Ord. No.
Flat-bottomed long tubes inclusive screw caps for MColortest™ with color-card comparator (1 pack = 12 pcs)	1.14901.0001
Flat-bottomed tubes inclusive screw caps for titrimetric and colorimetric MColortest™ (1 pack = 12 pcs)	1.14902.0001
Flat-bottomed tubes inclusive screw caps for MColortest™ with color-disk comparator (1 pack = 12 pcs)	1.17988.0001
Test vessels with 5 mL und 10 mL graduations, for MColortest™ and MQuant™ Tests (1 pack = 30 pcs)	1.17989.0001

Quality assurance

We check and calibrate our tests using certified buffer solutions, which can be traced directly to primary reference materials from NIST and PTB.

MColortest™ Compact Laboratory for Water Testing | Ord. No. 1.11151.0001

Determination of pH, ammonium, biological oxygen demand (BOD), carbonate hardness, total hardness, residual hardness, nitrate, nitrite, phosphate and oxygen.

This compact laboratory allows you to quickly measure all major parameters of standing or flowing surface water, and accurately assess the current water quality.

Scope of delivery

Parameter	Measuring range	No. of tests	Ord. No. Refill pack
MColortest™ Ammonium Test	0.2 – 5 mg/L NH_4	50	1.08024.0001
MColortest™ Carbonate Hardness Test / Acid cap. to pH 4.3 (ANC)	0.25 – 25 °e ANC: 0.1 – 7.2 mmol/L	150 at 12.5 °e	1.08048.0001
MColortest™ Total Hardness Test	0.25 °e and 10 mg/L	150 at 12.5 °e	1.08039.0001
MColortest™ Nitrate Test	10 – 150 mg/L NO_2	100	1.11170.0001
MColortest™ Nitrite Test	0.025 – 0.5 mg/L NO_2	200	1.08025.0001
MColortest™ pH Test	pH 4.5 – 9	200	1.08027.0001
MColortest™ Phosphate Test in freshwater and seawater	0.25 – 3.0 mg/L PO_4	100	1.14661.0001
MColortest™ Oxygen Test	0.1 mg/L O_2	100 at 8.5 mg/L O_2	1.11107.0001
Flat-bottomed tubes inclusive screw caps for MColortest™ Tests		3 pcs	
Thermometer			
Test vessels with 5 mL graduation		1 pc	



SCREEN ON THE GO

What is the quality
of your milk?

Detect peroxidase activity in milk

The application

- The quality of milk depends decisively on its successful heat treatment.
- If milk is heated to above 85° C, the enzyme lactoperoxidase (POD) is completely inactivated.
- The ultrahigh temperature control (UHT) of the milk can thus be documented.
- When lactoperoxidase is detected, pasteurization temperatures have been maintained and milk has been successfully pasteurized.
- For dairies, a yes / no statement is usually sufficient.

Our solution: MQuant™ Peroxidase test strips

With the qualitative MQuant™ Peroxidase Test, you can now determine the enzyme from your milk sample quickly and cost-effectively, instead of the more time-consuming photometry, and thus prove that their milk has been gently heated.

The test works just as reliably but significantly faster than the photometric reference method (DIN 10483-1). The rapid test is handy and can be used flexibly, directly at the sampling site.

Benefits

- Easy determination of peroxidase activity in milk
- Flexible application directly at the sampling site
- Low cost, low time requirement
- Easy evaluation with a color scale, whether activity is present

Learn more at: www.merckmillipore.com/aaf





Test strips
MQuant™

General information	140
What is the glucose content of your food?	140
Your brand – our test strips	143
MQuant™ test strips	144
Reagent papers	146



Test strips

Highly reliable and portable, **MQuant™** test strips are designed for semi-quantitative determination of ions and compounds. These versatile strips can be used in concentration ranges as low as below 1 mg/L up to the g/L range.

The test strips save you considerable time and costs during analyses, quality checks and in-process controls. Thanks to the PET film backing material and the low reagent content, the test strips are also easy to dispose of.



What is the glucose content of your food?

Semi-quantitative measurement of glucose

The application

- Glucose is an important parameter in many foods and beverages, and is regularly tested in raw materials and final products.
- Traditional glucose analysis involves time-consuming enzymatic determination in laboratories.

Our solution: MQuant™ Glucose test strips

MQuant™ Glucose test strips allow fast, cost-effective analysis anywhere. They deliver reliable semi-quantitative results, and are ideal for quick on-the-spot screening of samples when there's no time for lab analysis.

Benefits

- Pocket-sized tests for on-site or laboratory use
- Easy disposal
- Simple analysis with illustrated instructions on label
- Fast, accurate results in minutes
- Cost-effective solution

For more applications, please visit: www.merckmillipore.com/aaf

Fast,
easy, safe

Fast results, easy usage, safe disposal

Brilliant
color scales for
exact results

All for you ...

All concentration ranges available



Further MQuant™ applications

Check the quality of frying oils

Deep-frying causes oils and fats to decompose over time, producing free fatty acids. When these acids exceed an acceptable limit, they affect the quality of fried food. With MQuant™ Free Fatty Acids visual test strips, you can easily monitor the quality of your oil and determine the right time for a change. (MQuant™ Free Fatty Acids | Ord. No. 1.17046.0001)



Ensure safety after disinfection

Residues from disinfectants used in food production, hospitals, and biotech or pharmaceutical environments can cause serious problems. MQuant™ test strips help you monitor the cleaning process by checking for effective concentrations of disinfectants. We offer tests for: chlorine, formaldehyde, peracetic acid, peroxide and quaternary ammonium compounds.



It's that simple!

01 Sample preparation

The MQuant™ Test contains all necessary reagents, including those required for sample pre-treatment.



02 Testing



Remove one MQuant™ test strip from the protective tube.



Dip strip into the test solution to wet reaction zones. Remove excess liquid by shaking test strip or drawing it across the edge of the vessel.



After the specified reaction time (maximum one minute), compare the color of the reaction zone with the color scale printed on the tube label to determine the concentration.

03 Disposal

MQuant™ test strips can be safely and easily disposed of with regular waste.

Shelf-life and storage

When stored in a cool (refrigeration is necessary in some cases) and dry area, the test strips can be used up to three years (details printed in the pack). The tube must be closed immediately after removal of each strip to ensure the remaining test strips are protected.

Quality assurance

We check and calibrate all MQuant™ tests and comparison colors using certified standard solutions. These solutions can be traced directly to primary reference materials from NIST and PTB.



Want to add your branding to our test strips or test tubes? Choose from the following options:

Single sealed test strips

Customized test strips are ideal for inserting in books, magazines and brochures, or for adhering to products.

Tubes with list items or tailor-made test strips

Personalize almost anything, from the design of the color card to the final product, and even the measuring range.

Innovative customized products

If the test you need is not offered, we'll produce tailor-made test strips to suit your individual requirements.

To find out about our minimum quantity requirements, and for more details, please visit: www.merckmillipore.com/customized-test-strips

Your brand – our test strips

	Parameter	Graduation	No. of tests	Ord. No.	Method	Type
A	Aluminium Test	10–25–50–100–250 mg/L Al	100	1.10015.0001	Aurintricarboxylic acid	Reagent, incl.
	Ammonium Test	10–30–60–100–200–400 mg/L NH ₄	100	1.10024.0001	Neßler	Reagent, incl.
	Arsenic Test	0.005–0.010–0.025–0.05–0.10–0.25–0.5 mg/L As	100	1.17927.0001	modified Gutzeit test	Reagent, incl.
	Arsenic Test	0.02–0.05–0.1–0.2–0.5 mg/L As 0.1–0.5–1.0–1.7–3.0 mg/L As	100	1.17917.0001	modified Gutzeit test	Reagent, incl.
	Ascorbic Acid Test	50–100–200–300–500–700– 1,000–2,000 mg/L ascorbic acid	100	1.10023.0001	Phosphomolybdenum blue	
B	Blank strip		100	1.11860.0001		
C	Calcium Test	10–25–50–100 mg/L Ca	60	1.10083.0001	Glyoxal-bis-hydroxyanil	Reagent, incl.
	Carbonate Hardness Test	5–10–15–20–30 °e	100	1.10648.0001	Mixed indicator	
	Chloride Test	500–1,000–1,500–2,000–≥3,000 mg/L Cl	100	1.10079.0001	Silver chromate	
	Chlorine Test (free chlorine)	0.5–1–2–5–10–20 mg/L Cl ₂	75	1.17925.0001	Redox reaction	
	Chlorine Test (free chlorine)	25–50–100–200–500 mg/L Cl ₂	100	1.17924.0001	Redox reaction	
	Chromate Test	3–10–30–100 mg/L CrO ₄	100	1.10012.0001	Diphenylcarbazide	Reagent, incl.
	Cobalt Test	10–30–100–300–1,000 mg/L Co	100	1.10002.0001	Rhodanide	
	Copper Test	10–30–100–300 mg/L Cu	100	1.10003.0001	2,2'-Biquinoline	
	Cyanide Test	1–3–10–30 mg/L CN	100	1.10044.0001	König reaction	Reagent, incl.
F	Formaldehyde Test	10–20–40–60–100 mg/L HCHO	100	1.10036.0001	Triazole	Reagent, incl.
	Free Fatty Acids	0.5–1.0–2.0–3.0 mg/g KOH	100	1.17046.0001	pH indicator	
G	Glucose Test	10–25–50–100–250–500 mg/L Glucose	50	1.17866.0001	Enzymatic reaction	
I	Iron Test	3–10–25–50–100–250–500 mg/L Fe(II)	100	1.10004.0001	2,2'-Bipyridine	
L	Lead Test	20–40–100–200–500 mg/L Pb	100	1.10077.0001	Rhodizonic acid	Reagent, incl.
M	Manganese Test	2–5–20–50–100 mg/L Mn	100	1.10080.0001	Oxidation/Redox indicator	Reagent, incl.
	Molybdenum Test	5–20–50–100–250 mg/L Mo	100	1.10049.0001	Toluene-3,4-dithiol	Reagent, incl.
N	Nickel Test	10–25–100–250–500 mg/L Ni	100	1.10006.0001	Dimethylglyoxime	
	Nitrate Test	10–25–50–100–250–500 mg/L NO ₃	100	1.10020.0001	modified Griess' reaction	
	Nitrate Test	10–25–50–100–250–500 mg/L NO ₃	25	1.10020.0002	modified Griess' reaction	
	Nitrate Test	10–25–50–100–250–500 mg/L NO ₃	1,000	1.10092.0021	modified Griess' reaction	Individually sealed
	Nitrite Test	0.5–1–2–5–10 mg/L NO ₂	75	1.10057.0001	Griess' reaction	
	Nitrite Test	2–5–10–20–40–80 mg/L NO ₂	100	1.10007.0001	Griess' reaction	
	Nitrite Test	2–5–10–20–40–80 mg/L NO ₂	25	1.10007.0002	Griess' reaction	
	Nitrite Test	0.1–0.3–0.6–1–2–3 g/L NO ₂	100	1.10022.0001	Griess' reaction	
	Nitrite Test	0.1–0.3–0.6–1–2–3 g/L NO ₂	100	1.10022.0001	Griess' reaction	
P	Peracetic Acid Test	5–10–20–30–50 mg/L Peracetic acid	100	1.10084.0001	Redox reaction	
	Peracetic Acid Test	20–40–80–120–160 mg/L Peracetic acid	100	1.17976.0001	Redox reaction	
	Peracetic Acid Test	100–150–200–250–300–400–500 mg/L Peracetic acid	100	1.10001.0001	Redox reaction	
	Peracetic Acid Test	500–1,000–1,500–2,000 mg/L Peracetic acid	100	1.17922.0001	Redox reaction	
	Peroxidase Test	yes/no result	100	1.17828.0001	Enzymatic reaction	

	Beer processing	Food testing	Juices	Milk products	Mineral water	Soft drinks	Aquaculture	Boiler water, cooling water	Drinking water	Groundwater, surface water	Industrial water	Process water	Seawater	Swimming pools	Wastewater	Agriculture	Disinfection control	Electroplating	Parameter
	Food and beverages						Water (Analytics)								Others				
																			Aluminium Test
																			Ammonium Test
																			Arsenic Test
																			Arsenic Test
																			Ascorbic Acid Test
																			Blank strip
																			Calcium Test
																			Carbonate Hardness Test
																			Chloride Test
																			Chlorine Test
																			Chlorine Test
																			Chromate Test
																			Cobalt Test
																			Copper Test
																			Cyanide Test
																			Formaldehyde Test
																			Free Fatty Acids
																			Glucose Test
																			Iron Test
																			Lead Test
																			Manganese Test
																			Molybdenum Test
																			Nickel Test
																			Nitrate Test
																			Nitrate Test
																			Nitrate Test
																			Nitrite Test
																			Nitrite Test
																			Nitrite Test
																			Nitrite Test
																			Nitrite Test
																			Peracetic Acid Test
																			Peracetic Acid Test
																			Peracetic Acid Test
																			Peracetic Acid Test
																			Peroxidase Test

	Parameter	Graduation	No. of tests	Ord. No.	Method	Type
P	Peroxide Test	0.5–2–5–10–25 mg/L H ₂ O ₂	100	1.10011.0001	Enzymatic reaction	
	Peroxide Test	0.5–2–5–10–25 mg/L H ₂ O ₂	25	1.10011.0002	Enzymatic reaction	
	Peroxide Test	1–3–10–30–100 mg/L H ₂ O ₂	100	1.10081.0001	Enzymatic reaction	
	Peroxide Test	100–200–400–600–800–1,000 mg/L H ₂ O ₂	100	1.10337.0001	Enzymatic reaction	
	Phosphate Test	10–25–50–100–250–500 mg/L PO ₄	100	1.10428.0001	Molybdate ion	Reagent, incl.
	Potassium Test	250–450–700–1,000–1,500 mg/L K	100	1.17985.0001	Dipicrylamine	Reagent, incl.
Q	Quaternary Ammonium Compounds	10–25–50–100–250–500 mg/L Benzalkonium chloride	100	1.17920.0001	Indicator	
S	Sulfate Test	<200–>400–>800–>1200–>1600 mg/L SO ₄	100	1.10019.0001	Ba-thorin complex	
	Sulfite Test	10–40–80–180–400 mg/L SO ₃	100	1.10013.0001	Nitroprusside/ Zn-hexacyanoferrate	
T	Tin Test	10–25–50–100–200 mg/L Sn	50	1.10028.0001	Toluene-3,4-dithiol	Reagent, incl.
	Total Hardness Test	<4–>5–>9–>18–>26 °e	100	1.10025.0001	EDTA	
	Total Hardness Test	<4–>5–>9–>18–>26 °e	5,000	1.10029.0001	EDTA	Single test strips
	Total Hardness Test	<4–>5–>9–>18–>26 °e	1,000	1.10032.0001	EDTA	Individually sealed
	Total Hardness Test	>6–>13–>19–>25–>31 °e	100	1.10046.0001	EDTA	
	Total Hardness Test	>6–>13–>19–>25–>31 °e	25,000	1.10047.0013	EDTA	Individually sealed
	Total Hardness Test	<1.5; 1.5–2.5; >2.5 mmol/L CaCO ₃	100	1.17934.0001	EDTA	
Z	Zinc Test	0–4–10–20–50 mg/L Zn	100	1.17953.0001	Dithizone	

Reagent papers

Lead(II) acetate paper 3 rolls, each 4.8 meters

Ord. No. 1.09511.0003

Lead(II) acetate paper is used for the determination of sulfide and hydrogen sulfide

Potassium iodide-starch paper, grade value Reag. Ph Eur, 3 rolls, each 4.8 meters

Ord. No. 1.09512.0003

Potassium iodide-starch paper is used for the determination of oxidizing agents

	Beer processing	Food testing	Juices	Milk products	Mineral water	Soft drinks	Aquaculture	Boiler water, cooling water	Drinking water	Groundwater, surface water	Industrial water	Process water	Seawater	Swimming pools	Wastewater	Agriculture	Disinfection control	Electroplating	Parameter
	Food and beverages						Water (Analytics)						Others						
																			Peroxide Test
																			Peroxide Test
																			Peroxide Test
																			Peroxide Test
																			Phosphate Test
																			Potassium Test
																			Quaternary Ammonium Compounds
																			Sulfate Test
																			Sulfite Test
																			Tin Test
																			Total Hardness Test
																			Total Hardness Test
																			Total Hardness Test
																			Total Hardness Test
																			Total Hardness Test
																			Total Hardness Test
																			Zinc Test



blank zone control

MQuant™ Blank Test Strips include a reagent-free zone. This allows you to check whether the sample solution changes the color of the blank zone.



TAKE THE FAST TRACK

Having trouble
measuring the pH
of turbid samples?

Quick and clear pH measurements of turbid solutions

The application

- Analyzing turbid or colored liquids with conventional pH-indicator strips can be extremely difficult.
- Suspended particulate matter which accumulates on the reaction zone can obscure the color and make the pH impossible to read.
- Using pH electrodes leads to extensive cleaning and maintenance.

Our solution: MColorpHast™ non-bleeding pH-indicator strips

Our transparent pH-indicator strips for turbid solutions eliminate the need for sample preparation steps, such as filtration or clarification. The pH reaction zone is backed by a transparent carrier film, so you can easily read the pH on the reverse side of it.

Benefits

- Non-bleeding strips prevent contamination of the medium
- Transparent strips for clear results in lightly colored or turbid liquids
- Quick and easy method without sample preparation
- Brilliant color scales ensure reliable results
- SafetyEdge box for maximum security and convenience



pH test strips and papers

MColorpHast™

General information

150

SafetyEdge pink

150

pH test strips and papers

152



Food & beverage workflow
> Page 30

pH test strips and papers

MColorpHast™ makes pH measurement easier than ever. No instruments, sample preparation, maintenance, or cleaning electrodes. Simply read the color. The rapid method offers an accurate color scale for clear, reliable results. It's suitable for all types of media in environmental analysis and industrial in-process controls – even for highly turbid liquids. With our broad range of pH tests, you'll always have the optimal solution for your application.

SAFETYEDGE BOX



Performing pH measurements?

Enjoy the ultimate in security and simplicity with our SafetyEdge box. Its tamper-proof seal ensures that the box has not been opened, while its innovative flip-top corner allows easy removal of pH indicator strips, but prevents them from falling out.

Do you have special applications?

Simplify your workflow with our pH test strips for special requirements, like testing turbid samples or meat.

Food & beverage workflow
> Page 30



Read more about our pH test strips:
www.merckmillipore.com/pH-tests

Fast and
easy method

Non-bleeding
strips

Brilliant
colors

for convenient analysis

*With our broad range of pH tests,
you'll always have the optimal
solution for your application.*



Premium pH indicator papers

High-quality filter papers combined with a roll format, protect your tests from external factors, such as moisture, light, and ambient gases. This also ensures that they can be stored for a longer time.

MColorpHast™ non-bleeding pH indicator strips

Special indicator dyes are covalently bound to the reagent papers. This prevents the indicator from bleeding, and allows the strips to be left in the measurement medium indefinitely – without contaminating the sample.

pH-indicator papers

Product	pH measuring range	Graduation	Roll length / No. of strips	Ord. No.
Roll format				
pH-Box	0.5 – 13.0	0.5–1.0–1.5–2.0–2.5–3.0–3.5–4.0–4.5–5.0–5.5–6.0–6.5–7.0–7.5–8.0–8.5–9.0–9.5–10.0–10.5–11.0–11.5–12.0–12.5–13.0	3 x 4.8 m	1.09565.0001
pH-indicator paper Replacement rolls*	0.5 – 5.0	0.5–1.0–1.5–2.0–2.5–3.0–3.5–4.0–4.5–5.0	6 x 4.8 m	1.09568.0001
pH-indicator paper Replacement rolls*	5.5 – 9.0	5.5–6.0–6.5–7.0–7.5–8.0–8.5–9.0	6 x 4.8 m	1.09569.0001
pH-indicator paper Replacement rolls*	9.5 – 13.0	9.5–10.0–10.5–11.0–11.5–12.0–12.5–13.0	6 x 4.8 m	1.09570.0001
pH-indicator paper Universal indicator	1 – 14	1.0–2.0–3.0–4.0–5.0–6.0–7.0–8.0–9.0–10.0–12.0–14.0	3 x 4.8 m	1.10962.0003
pH-indicator paper Replacement rolls*	1 – 14	1.0–2.0–3.0–4.0–5.0–6.0–7.0–8.0–9.0–10.0–12.0–14.0	6 x 4.8 m	1.10232.0001
pH-indicator paper Universal indicator	1 – 10	1.0–2.0–3.0–4.0–5.0–6.0–7.0–8.0–9.0–10.0	3 x 4.8 m	1.09526.0003
pH-indicator paper Replacement rolls*	1 – 10	1.0–2.0–3.0–4.0–5.0–6.0–7.0–8.0–9.0–10.0	6 x 4.8 m	1.09527.0001
pH-indicator paper Acilit®	0.5 – 5.0	0.5–1.0–1.5–2.0–2.5–3.0–3.5–4.0–4.5–5.0	3 x 4.8 m	1.09560.0003
pH-indicator paper Replacement rolls*	0.5 – 5.0	0.5–1.0–1.5–2.0–2.5–3.0–3.5–4.0–4.5–5.0	6 x 4.8 m	1.09568.0001
pH-indicator paper Neutralit®	5.5 – 9.0	5.5–6.0–6.5–7.0–7.5–8.0–8.5–9.0	3 x 4.8 m	1.09564.0003
pH-indicator paper Replacement rolls*	5.5 – 9.0	5.5–6.0–6.5–7.0–7.5–8.0–8.5–9.0	6 x 4.8 m	1.09569.0001
pH-indicator paper Alkalit®	9.5 – 13.0	9.5–10.0–10.5–11.0–11.5–12.0–12.5–13.0	3 x 4.8 m	1.09562.0003
pH-indicator paper Replacement rolls*	9.5 – 13.0	9.5–10.0–10.5–11.0–11.5–12.0–12.5–13.0	6 x 4.8 m	1.09570.0001
pH-indicator paper Special indicator	3.8 – 5.4	<3.8–3.8–4.1–4.4–4.6–4.8–5.1–5.4	3 x 4.8 m	1.09555.0003
pH-indicator paper Special indicator	5.4 – 7.0	<5.4–5.4–5.8–6.2–6.4–6.7–7.0–>7.0	3 x 4.8 m	1.09556.0003
pH-indicator paper Special indicator	6.4 – 8.0	6.4–6.7–7.0–7.2–7.5–7.7–8.0–>8.0	3 x 4.8 m	1.09557.0003
pH-indicator paper Special indicator	8.2 – 10.0	<8.2–8.2–8.5–8.8–9.0–9.3–9.6–10.0	3 x 4.8 m	1.09558.0003
Litmus paper, blue Reag. Ph Eur	pH <4 red / >9 blue	–	3 x 4.8 m	1.09486.0003
Litmus paper, red Reag. Ph Eur	pH <4 red / >9 blue	–	3 x 4.8 m	1.09489.0003
Congo red paper Reag. Ph Eur	pH <2 blue-violet / >5 red-orange	–	3 x 4.8 m	1.09514.0003
Phenolphthalein paper	<8 colorless / >9 red	–	3 x 4.8 m	1.09521.0003
Booklet format				
pH-indicator paper Universal indicator	1 – 10	1.0–2.0–3.0–4.0–5.0–6.0–7.0–8.0–9.0–10.0	3 x 100	1.09525.0003

* Replacement roll without color scale

Shelf-life and storage

- Store at 10-25°C to maintain top condition for 3-5 years
- Protect from light and moisture
- Close box immediately after removing each strip or paper

pH-indicator strips (non-bleeding)

Product	pH measuring range	Graduation	No. of test strips	Ord. No.
pH-indicator strips Universal indicator	0 – 14	0-1-2-3-4-5-6-7-8-9-10-11-12-13-14	100	1.09535.0001
pH-indicator strips	0 – 6.0	0-0.5-1.0-1.5-2.0-2.5-3.0-3.5-4.0-4.5-5.0-5.5-6.0	100	1.09531.0001
pH-indicator strips	5.0 – 10.0	5.0-5.5-6.0-6.5-7.0-7.5-8.0-8.5-9.0-9.5-10.0	100	1.09533.0001
pH-indicator strips	7.5 – 14.0	7.5-8.0-8.5-9.0-9.5-10.0-10.5-11.0-11.5-12.0-12.5-13.0-13.5-14.0	100	1.09532.0001
pH-indicator strips	2.0 – 9.0	2.0-2.5-3.0-3.5-4.0-4.5-5.0-5.5-6.0-6.5-7.0-7.5-8.0-8.5-9.0	100	1.09584.0001
pH-indicator strips	0 – 2.5	0-0.5-1.0-1.3-1.6-1.9-2.2-2.5	100	1.09540.0001
pH-indicator strips	2.5 – 4.5	2.5-3.0-3.3-3.6-3.9-4.2-4.5	100	1.09541.0001
pH-indicator strips	4.0 – 7.0	4.0-4.4-4.7-5.0-5.3-5.5-5.8-6.1-6.5-7.0	100	1.09542.0001
pH-indicator strips	6.5 – 10.0	6.5-6.8-7.1-7.4-7.7-7.9-8.1-8.3-8.5-8.7-9.0-9.5-10.0	100	1.09543.0001
pH-indicator strips	11.0 – 13.0	11.0-11.5-11.8-12.1-12.3-12.5-12.8-13.0	100	1.09545.0001

pH-indicator strips (for professional use)

Product	pH measuring range	Graduation	No. of test strips	Ord. No.
pH-indicator strips Special indicator for pH-measurements in turbid solutions (suspensions)	2.0 – 9.0	2.0-3.0-4.0-5.0-6.0-7.0-8.0-9.0	100	1.09502.0001
pH-indicator strips Special indicator for pH-measurements in meat	5.2 – 7.2	5.2-5.6-6.0-6.4-6.8-7.2	100	1.09632.0001
pH-indicator strips, individually sealed	2.0 – 9.0	2.0-2.5-3.0-3.5-4.0-4.5-5.0-5.5-6.0-6.5-7.0-7.5-8.0-8.5-9.0	1,000	1.09450.0010
pH-indicator strips, individually sealed	2.0 – 9.0	2.0-2.5-3.0-3.5-4.0-4.5-5.0-5.5-6.0-6.5-7.0-7.5-8.0-8.5-9.0	25,000	1.09450.0013

! single sealed strips

Upon request, we offer individually sealed test strips for standard or special pH ranges. These can also be customized with your branding, making them ideal for inserting into magazines and brochures, or for adhering to your products.

www.merckmillipore.com/customized-test-strips



BE READY FOR ANYTHING

Get all the tools
you need for secure
analysis and monitoring.

From one trusted source.

We have everything you need for your workflow – from unique solutions for microbiological monitoring and chromatography to ultrapure water and a complete range of reagents and solvents. But that's not all we offer.

By combining our analytical and regulatory expertise, we ensure you have consistently accurate results supported by solid documentation. And by creating products and solutions that lower costs, increase efficiency, and make optimal use of resources, we help you boost productivity. So we don't only supply top-quality products for analysis, we give you complete peace of mind.

You can find a comprehensive overview of our product offers at:

www.merckmillipore.com

www.sigma-aldrich.com



Cooling & boiler water workflow
> Page 20



Wastewater workflow
> Page 22



Drinking water workflow
> Page 24



Bottled water workflow
> Page 26



Brewery workflow
> Page 28



Food & beverage workflow
> Page 30




Complementary products

Analysis and monitoring

Microbial and pathogen testing	156
Chromatography and inorganic reagents	158
Classical photometry and pesticide standards	160
Ingredients and nutritional testing	161
Water purification systems	163

Microbiological testing

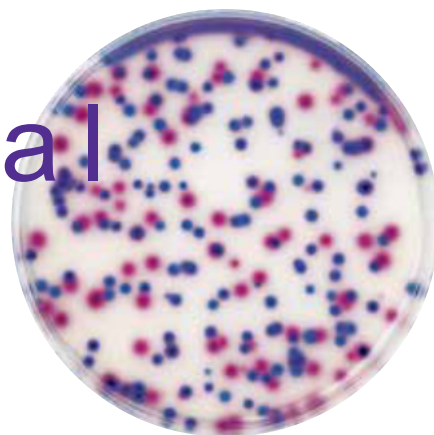

Easy, rapid and reliable tools
to ensure your production facilities
are free from microbiological contaminants

Rapidly verify the absence or presence of coliforms and *E. coli* with Readycult®

- USEPA approved for presence/absence detection of coliforms and *E. coli* in drinking water
- Optional 30-second indole test for accurate positive confirmation of *E. coli*
- **Readycult® Coliforms 100** [Ord. No. 1.01298.0001]
- **Readycult® Enterococci 100** [Ord. No. 1.01299.0001]

Screen any type of microbiological contamination

- **Chromocult®**: Separate color for each colony type ensures clear identification and easy counting [Ord. No. 1.10426.0500]
- **Ready-to-Use agar plates**: No additional preparation! [Ord. No. 1.46689.0020, 1.46757.0020 and 1.46758.0150]

bioburden analysis

Easily test bioburden in liquid samples with optimal microbiological recovery

- Comply with international standards (EP/USP) and water testing regulations
- **EZ-Fit™ Manifold, 1-, 3-, or 6-place Filtration Units** [Ord. No. EZFITEFUN1, EZFITEFUN3, EZFITEFUN6]
- **EZ-Fit™ Filtration Unit Membranes** [Ord. No. EFHAB100I, EFHAB250B, EFHAB250I, EFHAW100B, EFHAW100I, EFHAW250B, EFHAW250I]
- **EZ-Stream™ Pump** [Ord. No. EZSTREAM1]
- **EZ-Pak® Membranes** [e.g. Ord. No. EZAAWG474] for use with **EZ-Pak® Dispenser Curve** [Ord. No. EZCURVE01]



Surface Monitoring



Ensure hygiene through rapid testing

- **HY-LiTE® system:** Detect biological residues on surfaces and in process water [Ord. No. 1.30100.0301]
- **HY-RISE®:** Check for organic impurities on surfaces [Ord. No. 1.31200.0001]

Environmental Monitoring

Use our high-precision air samplers to easily and effectively monitor microorganisms in air and compressed gas.

- **MAS-100 Eco®:** for sterile environments and high risk food production areas [Ord. No. 1.09227.0001]
- **MAS-100 NT®:** Industry standard for routine air monitoring [Ord. No. 1.09191.0001]
- **MAS-100 Iso MH®:** Allows sampling 4 isolator points at once, each tube up to 10 m long [Ord. No. 1.17174.0001 or 1.17149.0001]
- **MAS-100 VF®:** Compact, portable design for varying sample locations [Ord. No. 1.17103.0001]
- **ARIES™ EX Dual Personal Sampling Pump:** Next-generation device with Bluetooth® compatibility and patented Mass Flow Controller [Ord. No. 30251-U]



analytical Chromatography

Do you need to separate the compounds in your sample, or require more detailed investigation? We offer a wide range of advanced chromatography and sample preparation products to support your application.

HPLC columns for different separations:

- **Chromolith®:** Low pressure, fast analysis, long column lifetime [Ord. No. 1.52022.0001]
- **Purospher® Star:** Excellent peak symmetry, high separation efficiency, extended pH stability, batch-to-batch reproducibility [Ord. No. 1.50359.0001]
- **SeQuant® ZIC®-HILIC** and **ZIC®-cHILIC:** Superior selectivity for separating polar hydrophilic compounds [Ord. No. 1.50441.0001]

High performance silica plates (HPTLC): for fast analysis of complex samples

Extrelut®: Effective liquid-liquid extraction (LLE)

LiChrolut®: Rapid and reliable solid-phase extraction (SPE)

Watercol™: Capillary gas chromatography (GC) columns for convenient measurement of water. Learn more: www.sigma-aldrich.com/watercol



reliable &
reproducible
separations

quantitation &
identification
of compounds

Inorganic reagents

Classical inorganic analysis



Salts



Acids



Caustic alkalis and bases



Metals and metal oxides

Instrumental inorganic analysis



Volumetric solutions



Karl Fischer reagents and standards



Reference materials



Fluxes for XRF



High purity acids and bases



High purity salts

Safety products and general applications



Absorption and filtration



Absorbents for spilled liquids



Drying agents



Auxiliaries for purification and sample preparation



Indicators



Cleaning applications

highest
quality

lowest
im purities

com pliant
with ACS &
Reag. Ph Eur

classical photometry

Inorganic analysis typically involves enrichment and isolation of trace elements prior to photometric determination. For both process steps, we offer an extensive range of high-quality reagents to make your analysis more efficient and economical from the start.

- **Carrez Clarification Kit for sample preparation in food analysis:**
Precipitate proteins, eliminate turbidity, break emulsions in meat or milk samples [Ord. No. 1.10537.0001]
- **Charcoal activated:** For de-colorization [Ord. No. 1.02005.0010]

Find the reagents
you need



efficient
& economical
analysis



Pesticide standards

Pesticides are released into the environment in order to kill pests. But residues from these toxic chemicals also end up in the air, water, and even in food. International regulations require regular analysis of soil and water using accurate standards to ensure that they are free of pesticides.

We offer more than 1700 high-purity pesticide standards and certified reference materials, including:

- Pesticides, neat and in solution
- Certified reference materials (CRM) TraceCERT® and matrix standards
- Matrix standards for proficiency testing (PT) (See page 106)
- Isotope-labeled pesticides and pesticide metabolite standards



Flavors & fragrances

Do you want to enhance the flavor and fragrance of your food? Or need to test these features? With our high-quality raw materials, analysis tools, reference materials and documentation, you can ensure your customers' safety and satisfaction.



Learn more:

www.sigmaaldrich.com/industries/flavors-and-fragrances.html



Nutrient analysis

Accurate information on protein and fiber content is needed for all food products. To simplify your work, we offer reliable kits for testing dietary fiber, and special reagents for Kjeldahl nitrogen analysis, which is the official method for determining protein content in food.

- **Reagent test kits for easy determination of total amount of dietary fiber**
[Ord. No. 1.12979.0001 and TDF100A]
- **Kjeldahl tablets for nitrogen determination**, also offered in micro-scale
[Ord. No. 1.15348.0250, 1.17958.0250, 1.16469.0250, 1.18348.0250, 1.10958.0250, 1.18469.0250]
- Learn more: www.merckmillipore.com/kjeldahl-catalysts



Brewery workflow
> Page 28



Food & beverage workflow
> Page 30



Karl Fischer reagents

It's important to measure water content in products because it can affect their quality, texture, shelf life, chemical stability and reactivity. Karl Fischer titration is a universally recognized method for determining water content in all types of substances, such as chemicals, oils, pharmaceuticals and food.

We offer all products required for Karl Fischer titration:

- **Volumetric reagents**
- **One-component reagents**
- **Two-component reagents:** special reagents for determining water in aldehydes, ketones and other substances that are difficult to solubilize
- **Coulometric reagents:** special solvents for oils and fats
- **Water standards** for titer determination and instrument monitoring



[Learn more](#)

food & beverage testing



Food & beverage workflow
> Page 30

Learn more about testing mycotoxins, antioxidants and carbohydrates on our "Food and Beverage Testing" webpage:

www.sigma-aldrich.com/industries/food-and-beverage.html

Water Purification systems

We offer a broad range of pure and ultrapure water purification systems for all lab applications. Our unique Milli-Q® system combines the most advanced technologies, such as intelligent RO, patented Elix® EDI, long-life UV, A10® TOC monitoring, and polishing cartridges – for best-in-class water purity.




Drinking water workflow
> Page 24

- **Water at your fingertips**
Q-POD® and E-POD® dispensers simplify operation and display essential data in an easy-to-use, compact device.
- **Facilitate your daily lab work**
Convenient, adaptable handling enables intuitive, precise dispensing. Select a specific volume with the autofill key or manually press the plunger.
- **Free up space on your bench**
As only the POD is needed for daily use, the system can be placed conveniently under the bench, or on the wall.
- **Get the right water quality for your application**
An Application-Pak on each POD provides final polishing to match water quality to your exact needs.



Discover our complete
lab water systems and services:
www.merckmillipore.com/labwater

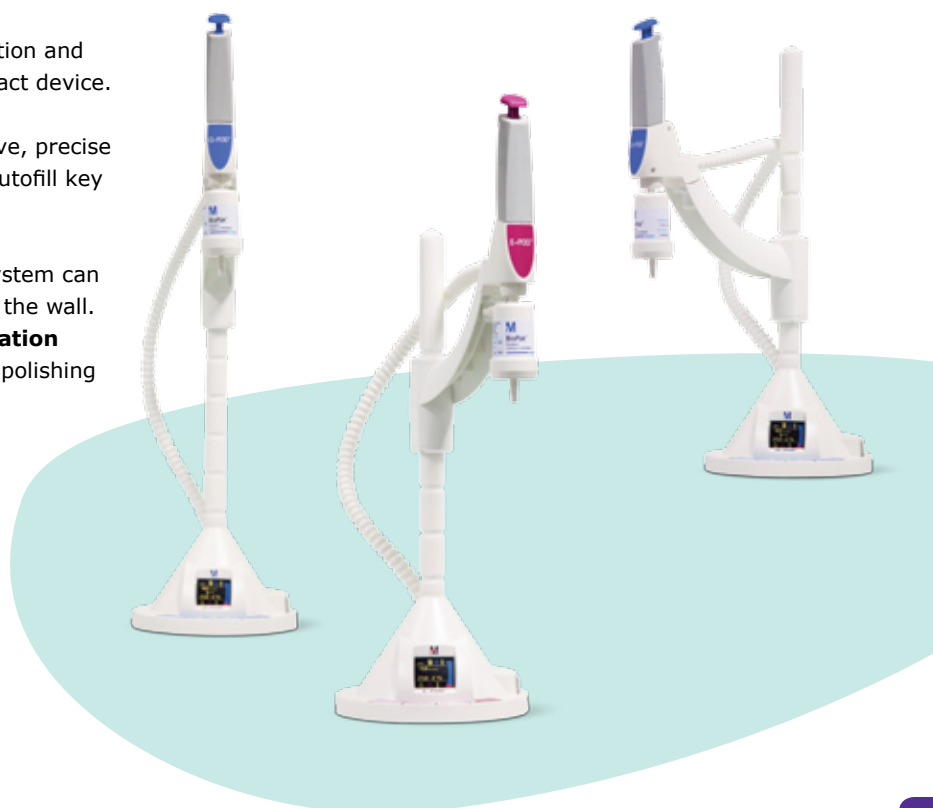

millex® syringe filters

- Superior quality and convenience for sensitive instrumental analyses, e.g. gas, liquid, or ion chromatography
- Low extractables and low analyte-binding membranes
- High chemical compatibility for use with almost any sample



Learn more



Ask for more

No matter where in the world you are, we're here to help. Whether you need product details, training courses, application advice or disposal tips, just ask.

A to Z

Service and information	Direct web address
A Analytical application notes finder More than 300 applications for Reflectoquant® and Spectroquant® test kits. • Get complete analytical procedures • Learn sample preparation methods • Determine measurement parameters • Compare the process with other methods • If you don't find the right application note for your specific application, please contact us	www.merckmillipore.com/aaf www.merckmillipore.com/support
B Brochures Stay up to date with our latest brochures, quick guides and other useful material.	www.merckmillipore.com/test-kits www.merckmillipore.com/learningcenter
C Certificates We provide lot certificates and certificates of quality for our products. Also see: ISO 14001 certificate	www.merckmillipore.com/wfa-documents
Consultancy and technical expert support Besides analytical and technical advice from our local specialists, we also offer immediate, expert support through hotlines in almost all countries.	www.merckmillipore.com/support
Customer support Get expert advice from your local customer service and technical support specialists.	www.merckmillipore.com/support www.sigma-aldrich.com/customer-service.html
D Direct access to product information Enter the six-digit product number into the search field to find usage instructions, applications, technical documents, brochures, accessories and related products.	www.merckmillipore.com www.sigma-aldrich.com

Service and information	Direct web address
E E-shop All our products for water, food, and environmental analytics and 350,000 more can be purchased online 24/7.	▶ www.sigma-aldrich.com
I Instrument support Contact your local customer support hotline. Also see: Service plan	▶ www.merckmillipore.com/support
ISO certificates • 57 of our production sites hold ISO 14001 Environmental Management certification • Internal and external audits are regularly performed at our production sites	▶ www.merckmillipore.com/iso
L Learning center • More about our products • How, when and where to use them	▶ www.merckmillipore.com/learningcenter
M Manuals Find detailed instruction manuals for all of our instruments and test kits in the respective product pages.	▶ www.merckmillipore.com/test-kits
Material Data Sheets and Certificates of Analysis Type in the batch number or article code, and get your documents in one click.	▶ www.merckmillipore.com/msds ▶ www.sigma-aldrich.com/msds
Mobile app center Apps for smartphones and tablets, e.g. "Food Testing" and "Industrial"	▶ www.merckmillipore.com/apps ▶ www.sigma-aldrich.com/mobileappcenter
O Online courses, webinars and webcasts Learn more online See also: Webinars, and Webcasts and videos	▶ www.merckmillipore.com/videos ▶ www.merckmillipore.com/webcasts
P Package inserts • Important handling information • Printed version is included in test kits, or can be downloaded from product detail pages	▶ www.merckmillipore.com/test-kits
Photometer method update • Update the software on your photometer to ensure its accuracy and compatibility with new tests. • This free service is available via the "Quick Links".	▶ www.merckmillipore.com/method-update
Product information See: Direct access to product information	▶ www.merckmillipore.com
R Research and development • New test kits are regularly developed to serve your needs • If you do not find the test kit or parameters you require, please contact us for further advice	▶ www.merckmillipore.com/support

Service

Ask for more

Service and information	Direct web address
R Return and recycle test kits See: Waste disposal advice	▶ www.disposal-test-kits.com
S Safety for personnel In developing our test kits, we avoid the use of harmful chemicals, such as chloroform, cadmium or benzene, wherever possible. We also supply comprehensive advice for safe waste disposal.	▶ www.merckmillipore.com/safety
Search online • Search by product name, product number or keyword. • As you type your search string, you will get suggestions in a drop-down list. • Choose from the list and you will be immediately directed to the corresponding product page.	▶ www.merckmillipore.com/test-kits ▶ www.sigma-aldrich.com
Service plan The Spectroquant® Service Plan minimizes breakdowns to maximize productivity. It includes: • Performance check with reference materials and certificates • Factory-recommended instrument maintenance • Support hotline • Free software upgrade • Reagent delivery program	▶ www.merckmillipore.com/water-analytics-service
Shipping of goods Strict international regulations are followed to ship your goods.	▶ www.merckmillipore.com/packaging
T Technical support See: Customer support	▶ www.sigma-aldrich.com/technical-service-home.html
Training courses and seminars • Our experts provide practical advice to help you avoid errors in your analysis, and give you tips and tricks to help towards accreditation • Small groups ensure that each participant receives optimum attention and instruction • Online webinars are available free of charge	▶ www.merckmillipore.com/learningcenter ▶ www.merckmillipore.com/support ▶ www.sigma-aldrich.com/customer-service.html
V Validation and accreditation for Spectroquant® test kits • All of the methods are validated • Certificate of quality and lot certificate to confirm quality • If you plan to validate Spectroquant® test kits or are applying for accreditation, please contact us to obtain documents created for approvals by organizations like the USEPA	▶ www.merckmillipore.com/wfa-documents
Visits and Demonstration on-site for support with presentations and demonstrations of handling of instruments and test kits in your laboratory please contact our customer service	▶ www.merckmillipore.com/support ▶ www.sigma-aldrich.com/customer-service.html

Service and information

Direct web address

W Waste disposal advice – online

Get clear instructions on how to properly dispose of used test kits. ► www.disposal-test-kits.com

Waste disposal service

Convenient service for safe disposal of chemical waste acc. to local legal requirements. For details and service, please contact your local account manager.

Webcasts and videos

Watch and learn about correct instrument usage and sample preparation techniques.

► www.merckmillipore.com/webcast_asp_wfa
 ► www.merckmillipore.com/video_asp_wfa

Webinars

Our webinars offer more detailed information about food, water, and environmental analysis.

► www.merckmillipore.com/webinars
 > Analytics and Sample Preparation
 ► www.sigma-aldrich.com/webinars

VISIT OUR E-SHOP ...



All our products for water, food and environmental analytics are available online – day or night. For further details and easy shopping, please visit

www.sigma-aldrich.com

24/7

Service

Product number index

Ready to get the best products for your water, food or environmental analysis? Use the index to find the product number, then visit our website to place your order. We wish you happy shopping and successful analyses. > www.sigma-aldrich.com

Cat. No.	Page	Cat. No.	Page	Cat. No.	Page	Cat. No.	Page	Cat. No.	Page	Cat. No.	Page
100...		100885	76	108161	90	109749	44	111...		114434	128
100049	60	100961	78	108163	90	109751	43	111103	128	114438	130
100086	62	101...		108164	90	109752	43	111104	134	114441	130
100087	62	101632	70	108165	90	109769	44	111106	128	114449	134
100088	62	101744	72	108166	90	109772	66	111107	132	114500	68
100089	62	101745	60	108203	134	109773	66	111109	128	114537	72
100474	72	101746	76	108312	134	109779	44	111110	128	114540	64
100475	74	101747	60	109...		110...		111117	128	114541	64
100594	58	101749	78	109450	153	110001	144	111122	134	114542	70
100595	62	101758	58	109486	152	110002	144	111131	132	114543	74
100597	62	101764	76	109489	152	110003	144	111132	128	114544	58
100598	62	101787	76	109502	153	110004	144	111136	130	114546	74
100599	62	101796	64	109511	146	110006	144	111138	134	114547	72
100602	62	101797	64	109512	146	110007	144	111142	134	114548	76
100605	60	101804	62	109514	152	110011	146	111143	130	114549	68
100606	68	101807	62	109521	152	110012	144	111148	134	114551	72
100607	72	101809	78	109525	152	110013	146	111151	137	114552	64
100608	62	101812	76	109526	152	110015	144	111152	132	114553	66
100609	72	101813	76	109527	152	110019	146	111157	130	114554	70
100613	72	101842	70	109531	153	110020	144	111160	130	114555	64
100614	70	101846	70	109532	153	110022	144	111169	132	114556	72
100615	74	102...		109533	153	110023	144	111170	132	114558	58
100616	74	102531	66	109535	153	110024	144	111174	130	114559	58
100617	76	102532	76	109540	153	110025	146	111860	144	114560	64
100673	74	102537	76	109541	153	110028	146	114...		114561	66
100675	58	102552	76	109542	153	110029	146	114394	76	114562	74
100677	58	104...		109543	153	110032	146	114400	128	114563	70
100678	58	104660	90	109545	153	110036	144	114401	128	114564	76
100680	60	107...		109555	152	110044	144	114402	130	114566	78
100683	58	107302	118	109556	152	110046	146	114403	130	114598	68
100687	60	108...		109557	152	110047	146	114404	132	114622	78
100688	60	108017	130	109558	152	110049	144	114406	132	114651	130
100718	60	108018	130	109560	152	110057	144	114408	132	114652	134
100784	44	108023	130	109562	152	110077	144	114410	134	114653	128
100787	44	108024	128	109564	152	110079	144	114411	134	114657	128
100796	68	108025	132	109565	152	110080	144	114412	134	114658	132
100798	74	108027	132	109568	152	110081	146	114413	128	114660	130
100809	68	108028	130	109569	152	110083	144	114414	130	114661	134
100815	70	108033	134	109570	152	110084	144	114416	134	114662	132
100816	70	108038	132	109584	153	110092	144	114417	130	114663	132
100822	68	108039	134	109632	153	110232	152	114418	130	114667	44
100826	60	108040	134	109701	66	110337	146	114420	132	114669	134
100856	72	108043	132	109711	68	110428	146	114421	130	114670	128
100857	76	108046	134	109713	70	110648	144	114423	128	114675	99
100858	62	108047	134	109717	68	110653	136	114424	132	114676	98
100860	70	108048	128	109734	44	110654	136	114428	128	114678	68
100861	78	108160	90	109748	43	110962	152	114429	130	114683	74

Cat. No.	Page	Cat. No.	Page	Cat. No.	Page	Cat. No.	Page	Cat. No.	Page	Cat. No.	Page
114687	51	114846	134	116993	120	118458	130	125038	105	133012	104
114688	51	114848	72	116995	120	118459	130	125039	105	133013	104
114689	100	114878	78	116996	120	118460	132	125040	105	133014	104
114690	64	114879	78	116997	120	118461	132	125041	105	133018	104
114691	64	114895	64	117...		118462	132	125042	105	133019	104
114693	89	114896	68	117046	144	118463	132	125043	105	133020	104
114694	72	114897	62	117048	64	118465	134	125044	105	133021	105
114695	99	114901	136	117058	64	118466	134	125045	105	133022	105
114696	100	114902	136	117059	64	118467	134	125046	105	133023	105
114724	44	114942	72	117179	128	118468	134	125047	105	133024	105
114729	74	114944	44	117828	144	118700	101	125048	105	171...	
114730	62	114946	44	117866	144	118701	101	125049	105	171200	53
114731	68	114947	44	117917	144	118750	80	125050	105	171201	53
114738	100	114962	89	117920	146	118751	80	125051	105	171202	53
114739	58	114963	89	117922	144	118752	80	125052	105	171203	53
114750	128	114964	44	117924	144	118753	80	125053	105	171204	53
114752	58	114976	128	117925	144	118754	130	132...		173...	
114753	128	114977	128	117927	144	118755	132	132225	104	173015	80
114756	130	114978	128	117934	146	118756	130	132226	104	173016	38
114758	64	114979	128	117942	120	118757	130	132227	104	173017	38
114759	130	115...		117945	120	118758	132	132228	104	173018	38
114761	68	115955	64	117952	120	118759	132	132229	104	173500	78
114763	72	116...		117953	146	118771	130	132230	104	173501	60
114764	70	116124	120	117956	120	118773	132	132231	104	173502	44
114765	130	116125	120	117961	120	118789	68	132233	104	173503	89
114767	66	116127	120	117963	120	119...		132234	104	173630	42
114768	132	116128	120	117968	120	119251	72	132235	104	173632	41
114770	70	116136	120	117976	144	119253	66	132236	104	173633	44
114773	70	116141	120	117985	146	119254	80	132237	104	173634	44
114774	132	116720	120	117988	136	119256	80	132238	104	173635	41
114776	72	116730	120	117989	136	119257	80	132239	104	173650	44
114777	134	116731	120	118...		119258	80	132240	105	174...	
114779	73	116732	120	118322	128	119301	89	132241	105	174010	44
114780	134	116892	120	118323	134	119302	89	132242	105	174011	44
114782	134	116894	120	118324	112	120...		132243	105	174064	44
114783	132	116896	120	118325	112	120097	44	132244	105		
114785	70	116898	120	118326	128	120347	44	132245	105		
114791	76	116899	120	118328	113	120497	44	132246	105		
114792	134	116953	118	118329	113	125...		132247	105		
114794	76	116954	118	118331	112	125022	104	132248	105		
114798	130	116957	118	118332	113	125023	104	132249	105		
114801	128	116970	118	118335	113	125024	104	132251	105		
114803	128	116971	120	118342	113	125025	104	132252	105		
114815	60	116973	120	118343	113	125026	104	132253	105		
114821	68	116974	120	118349	113	125027	104	133...			
114825	58	116975	120	118381	113	125028	104	133002	104		
114826	130	116976	120	118386	128	125029	104	133003	104		
114831	76	116977	120	118387	132	125030	104	133004	104		
114832	78	116978	120	118388	134	125031	104	133005	104		
114833	68	116981	120	118389	134	125032	104	133006	104		
114834	60	116982	120	118394	134	125033	104	133007	104		
114839	60	116983	120	118452	128	125034	104	133008	104		
114842	74	116987	120	118455	128	125035	104	133009	104		
114843	134	116989	120	118456	130	125036	105	133010	104		
114845	134	116992	120	118457	130	125037	105	133011	104		

NATURALLY THE BEST CHOICE

At Merck, we develop products that not only support our customers but also respect our planet. So while we constantly improve our tool kits, instruments and accessories to give you even greater precision in your analysis, we also continuously reduce the hazardous chemicals in our products to protect users and the environment. Naturally, this makes them the best choice for everyone.



www.merckmillipore.com/responsibility





Polyscientific Enterprise Sdn Bhd
百利企业有限公司 ^{152064 D}

Melaka (HQ)
272, Taman Asean,
Jalan Malim,
75250 Melaka

T +606 3350690 **F** +606 3351631

Shah Alam
14, Jalan Serendah 26/39,
Kawasan Perindustrian HICOM,
40400 Shah Alam, Selangor

T +603 51036920 **F** +603 51036980

Penang
16, Jalan Sungai Tiram 7,
11900 Bayan Lepas,
Penang

T +604 6371500 **F** +604 6371600

Johor
No. 365 Jalan Ekoperniagaan 11,
Taman Ekoperniagaan 2,
Senai Airport City, 81400 Senai,
Johor

T +607 5955243 **F** +607 5998822

info@polyscientific.com.my

www.poly.my